

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102424\
 Data File : BP022583.D
 Acq On : 24 Oct 2024 11:40
 Operator : RC/JU
 Sample : PB164325BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	41	rBV	24204	31548	1.05%	0.105%
2	3.605	101	105	123	rBV	290448	468334	15.64%	1.563%
3	3.916	154	158	167	rVB2	13208	19234	0.64%	0.064%
4	6.799	641	648	649	rBV5	4119	6029	0.20%	0.020%
5	6.846	649	656	668	rVB	399114	634388	21.19%	2.117%
6	6.993	674	681	692	rVB	299142	467160	15.60%	1.559%
7	7.193	705	715	726	rBV	389759	636418	21.25%	2.124%
8	7.652	785	793	801	rBV	420257	643844	21.50%	2.149%
9	8.352	904	912	927	rBV	472218	803582	26.84%	2.682%
10	8.793	979	987	996	rBV	389160	637617	21.29%	2.128%
11	9.199	1049	1056	1060	rBV4	6729	10486	0.35%	0.035%
12	9.504	1098	1108	1117	rBV	337606	563933	18.83%	1.882%
13	10.040	1190	1199	1213	rBV	498043	862778	28.81%	2.880%
14	10.404	1251	1261	1277	rBV	497984	884140	29.53%	2.951%
15	10.546	1277	1285	1306	rBV	421345	821161	27.42%	2.741%
16	11.216	1392	1399	1401	rBV8	1843	3337	0.11%	0.011%
17	11.675	1471	1477	1483	rBV5	6043	10415	0.35%	0.035%
18	11.998	1524	1532	1536	rBV3	9106	14958	0.50%	0.050%
19	13.669	1810	1816	1828	rBV	1079828	1406370	46.97%	4.694%
20	13.957	1852	1865	1874	rBV	1095251	1525736	50.95%	5.093%
21	14.110	1887	1891	1893	rBV4	3033	3825	0.13%	0.013%
22	14.269	1910	1918	1925	rBV	922560	1371554	45.80%	4.578%
23	14.504	1950	1958	1978	rBV	301552	690259	23.05%	2.304%
24	14.692	1986	1990	1994	rVB7	4162	5857	0.20%	0.020%
25	15.281	2082	2090	2098	rBV	1370154	2010297	67.13%	6.710%
26	15.404	2105	2111	2124	rBV	499016	683666	22.83%	2.282%
27	15.516	2127	2130	2135	rVB4	7586	11439	0.38%	0.038%
28	15.851	2183	2187	2190	rBV6	2195	3368	0.11%	0.011%
29	16.075	2222	2225	2230	rVB7	4689	8142	0.27%	0.027%
30	16.392	2277	2279	2282	rVB4	4124	4028	0.13%	0.013%
31	16.445	2284	2288	2295	rBV10	2882	6239	0.21%	0.021%
32	16.733	2335	2337	2344	rVB8	3055	4768	0.16%	0.016%
33	16.845	2353	2356	2360	rVB5	3502	5502	0.18%	0.018%
34	17.069	2388	2394	2403	rBV	1337121	1838277	61.39%	6.136%
35	17.163	2404	2410	2424	rVB	1603570	2297673	76.73%	7.669%
36	18.010	2549	2554	2563	rBV2	42022	78956	2.64%	0.264%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102424\
Data File : BP022583.D
Acq On : 24 Oct 2024 11:40
Operator : RC/JU
Sample : PB164325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	19.098	2734	2739	2744	rBV2	22690	38614	1.29%	0.129%
38	19.180	2749	2753	2757	rVV	22539	31653	1.06%	0.106%
39	19.351	2778	2782	2790	rBV9	28608	55537	1.85%	0.185%
40	19.557	2810	2817	2825	rBV	2187225	2928095	97.78%	9.773%
41	21.504	3142	3148	3160	rBV	1632841	2212860	73.90%	7.386%
42	24.557	3657	3667	3679	rVB	1044064	2994486	100.00%	9.995%
43	24.774	3695	3704	3715	rVB	871071	2223846	74.26%	7.423%




Sum of corrected areas: 29960409

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102424\
Data File : BP022583.D
Acq On : 24 Oct 2024 11:40
Operator : RC/JU
Sample : PB164325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

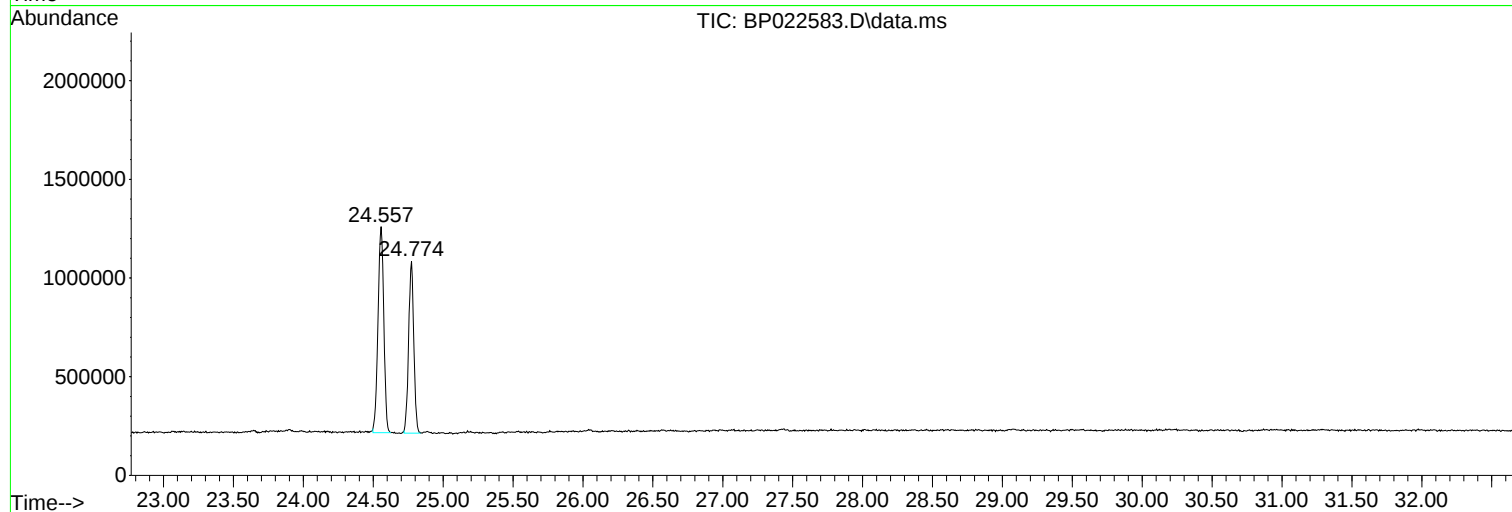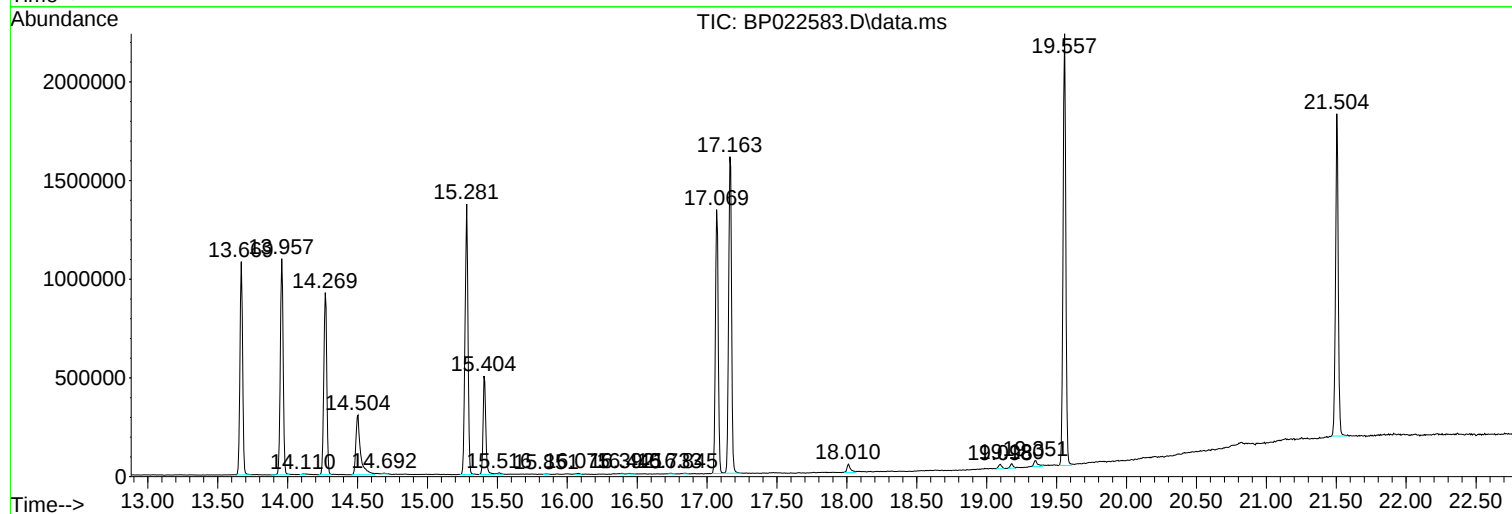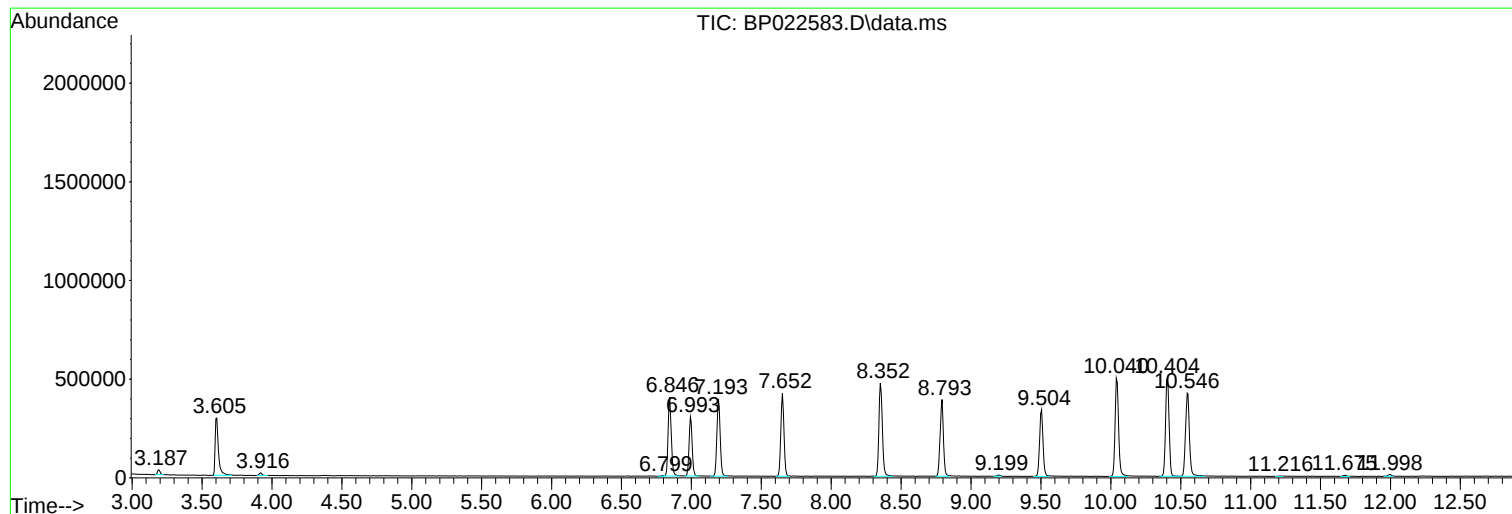

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102424\
Data File : BP022583.D
Acq On : 24 Oct 2024 11:40
Operator : RC/JU
Sample : PB164325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102424\
Data File : BP022583.D
Acq On : 24 Oct 2024 11:40
Operator : RC/JU
Sample : PB164325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc