




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102522\
 Data File : BP012321.D
 Acq On : 25 Oct 2022 18:45
 Operator : CG/JU
 Sample : SST08090
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080607

Manual IntegrationsAPPROVED

Quant Time: Oct 27 03:10:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/27/2022
 Supervised By :mohammad ahmed 10/27/2022

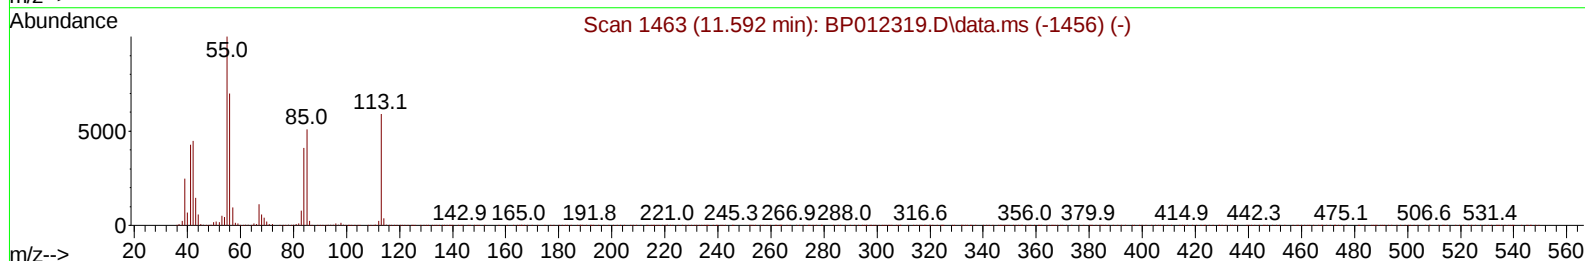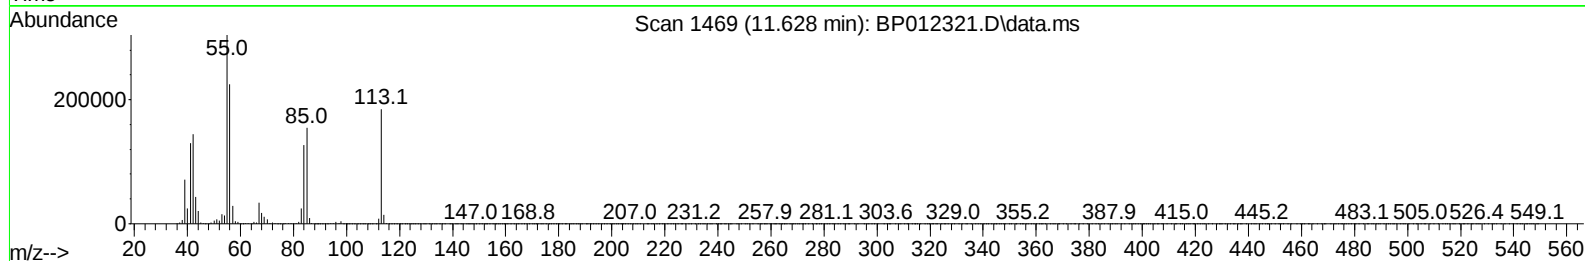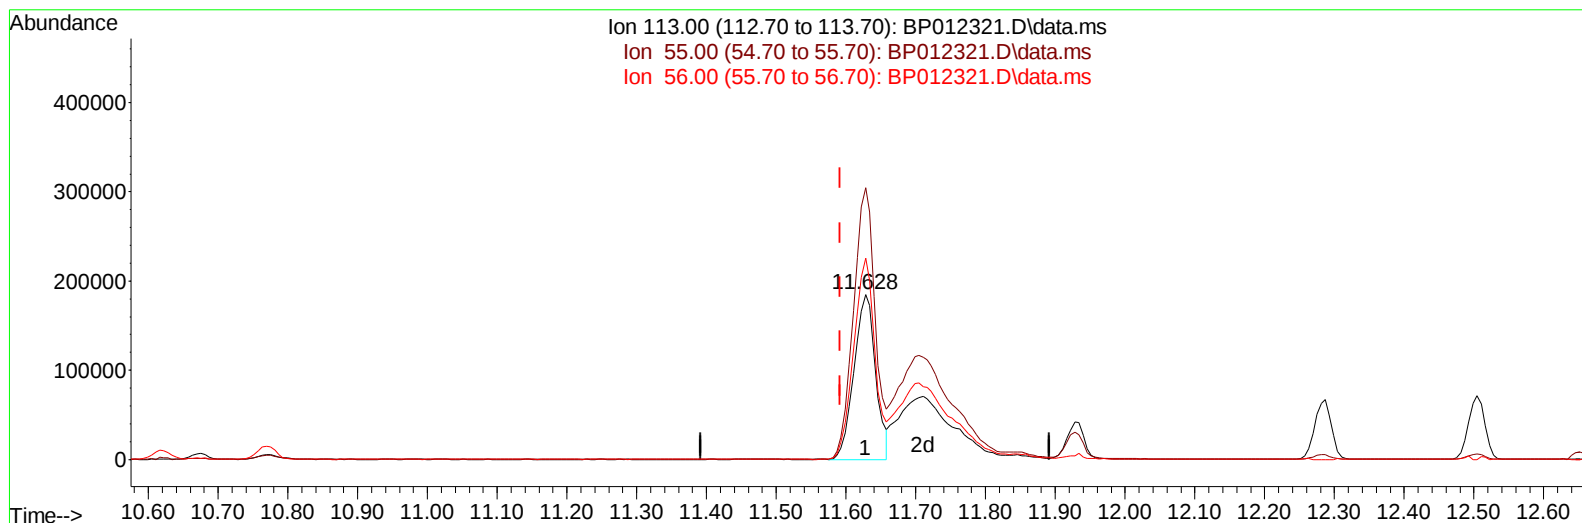

TIC: BP012321.D\data.ms

(34) Caprolactam

11.628min (+ 0.036) 43.72 ng/ul

response 395842

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	169.50	164.65
56.00	123.60	121.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102522\
Data File : BP012321.D
Acq On : 25 Oct 2022 18:45
Operator : CG/JU
Sample : SSTD08090
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD080607

Manual IntegrationsAPPROVED

Quant Time: Oct 26 10:08:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 10:05:01 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/27/2022
Supervised By :mohammad ahmed 10/27/2022

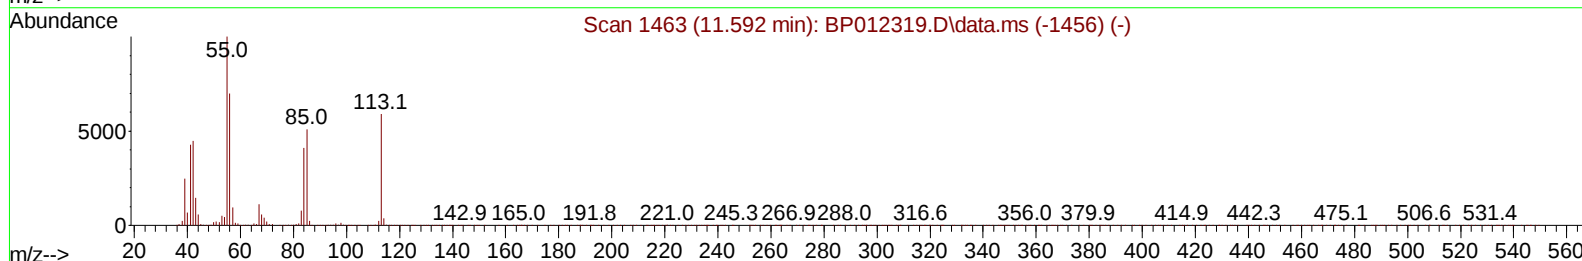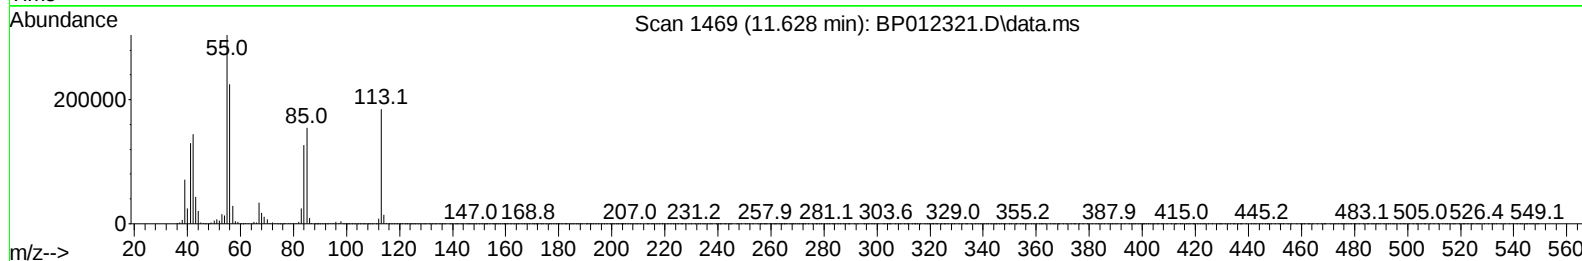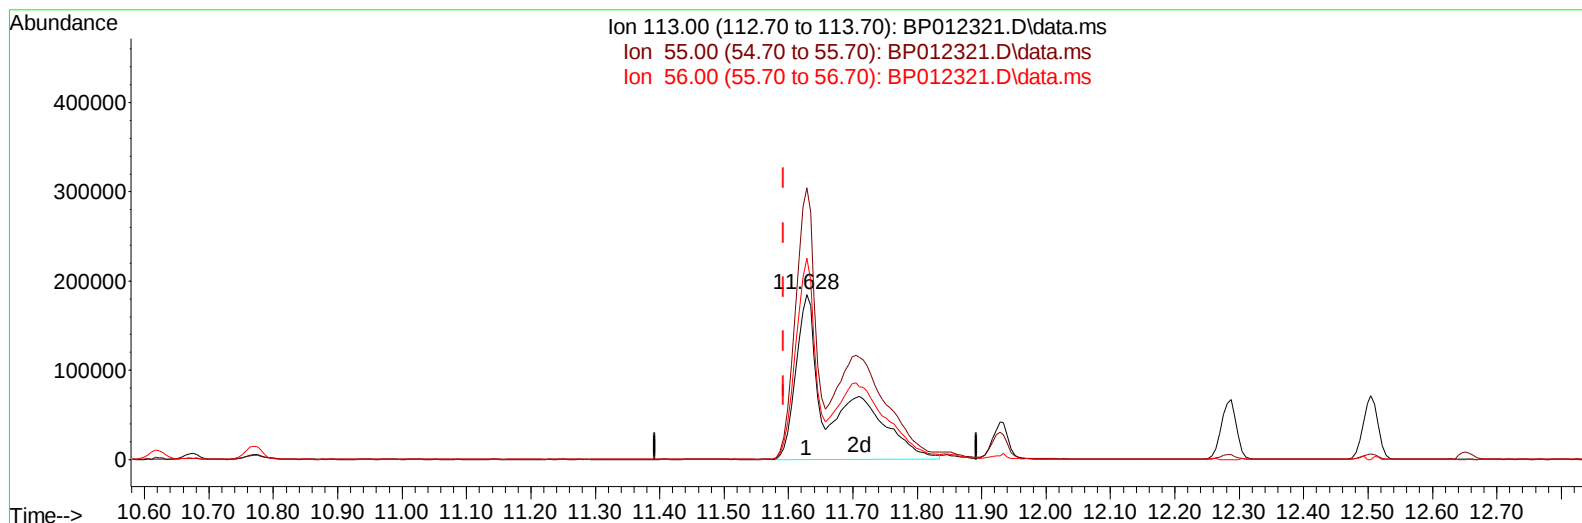

TIC: BP012321.D\data.ms

(34) Caprolactam

11.628min (+ 0.036) 91.60 ng/ul m

response 777381

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	170.00	164.65
56.00	118.70	121.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102522\
 Data File : BP012321.D
 Acq On : 25 Oct 2022 18:45
 Operator : CG/JU
 Sample : SST08090
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080607

Manual IntegrationsAPPROVED

Quant Time: Oct 27 03:10:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/27/2022
 Supervised By :mohammad ahmed 10/27/2022

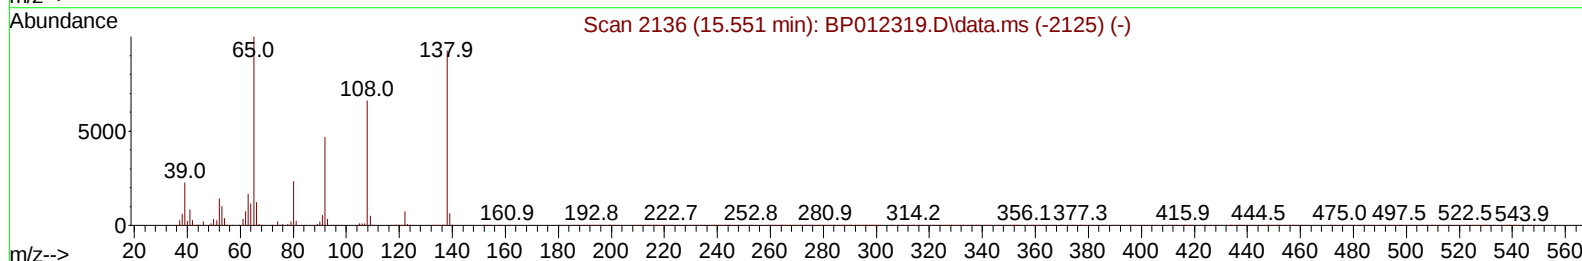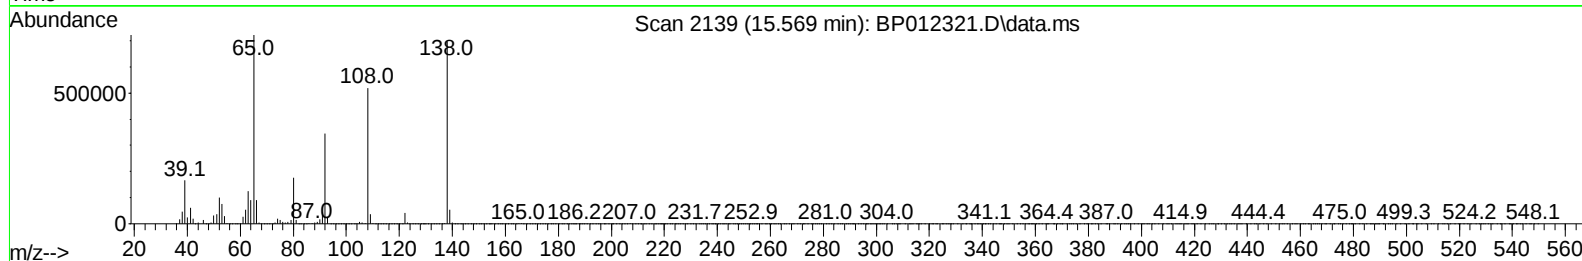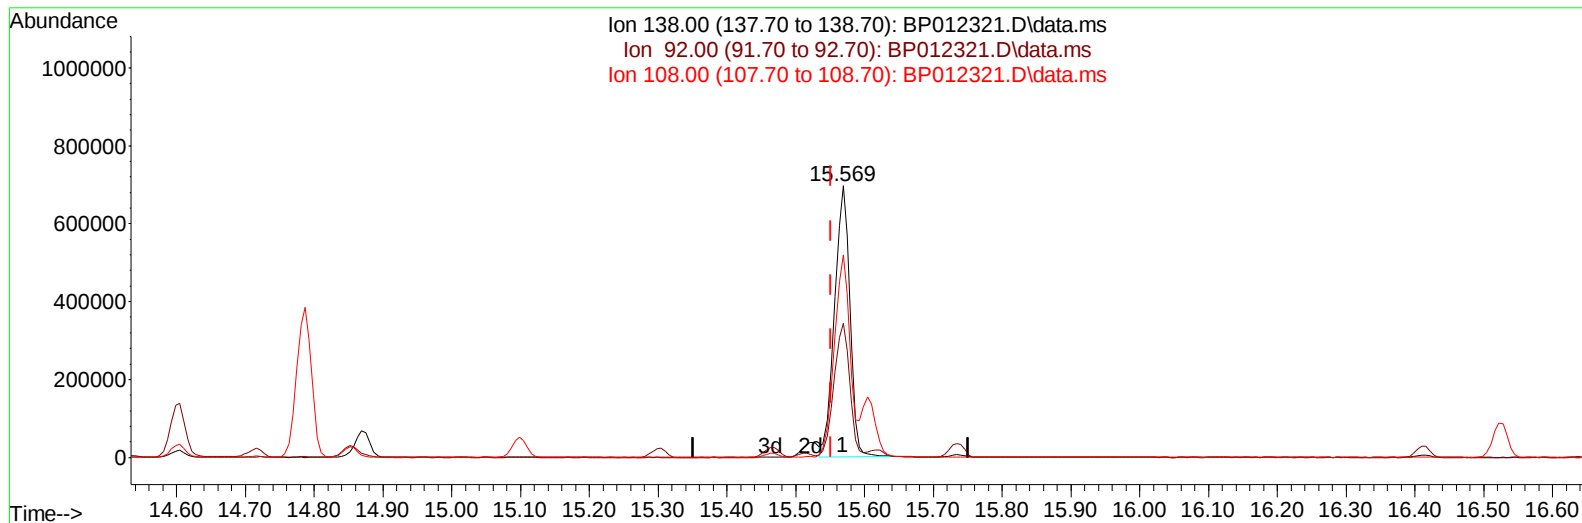

TIC: BP012321.D\data.ms

(63) 4-Nitroaniline

15.569min (+ 0.018) 77.74 ng/ul

response 1081059

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	50.80	49.44
108.00	70.80	74.58
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102522\
 Data File : BP012321.D
 Acq On : 25 Oct 2022 18:45
 Operator : CG/JU
 Sample : SST08090
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080607

Manual IntegrationsAPPROVED

Quant Time: Oct 26 10:08:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 10:05:01 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/27/2022
 Supervised By :mohammad ahmed 10/27/2022

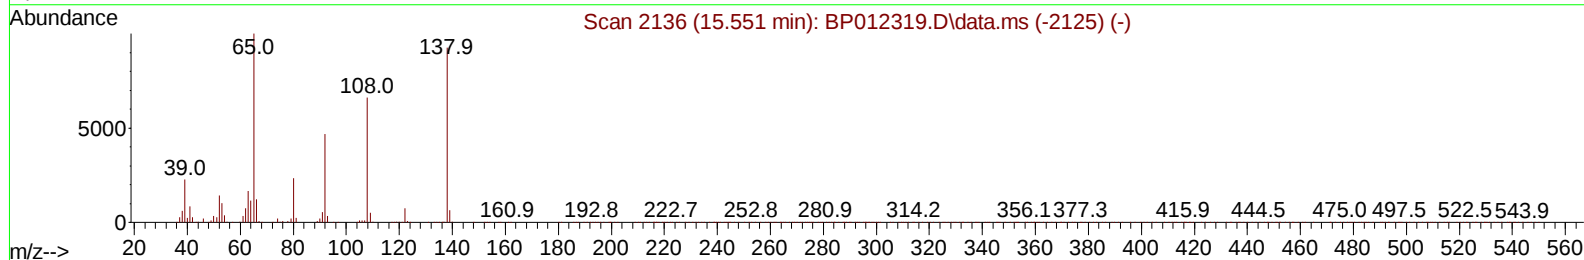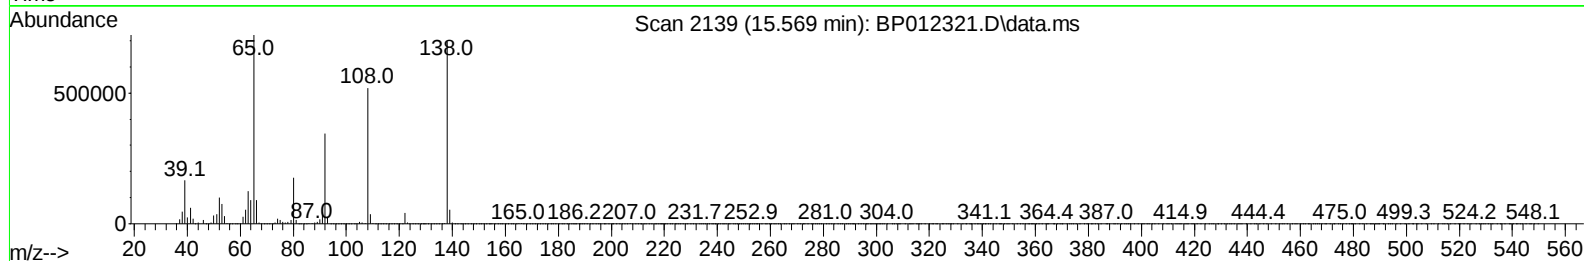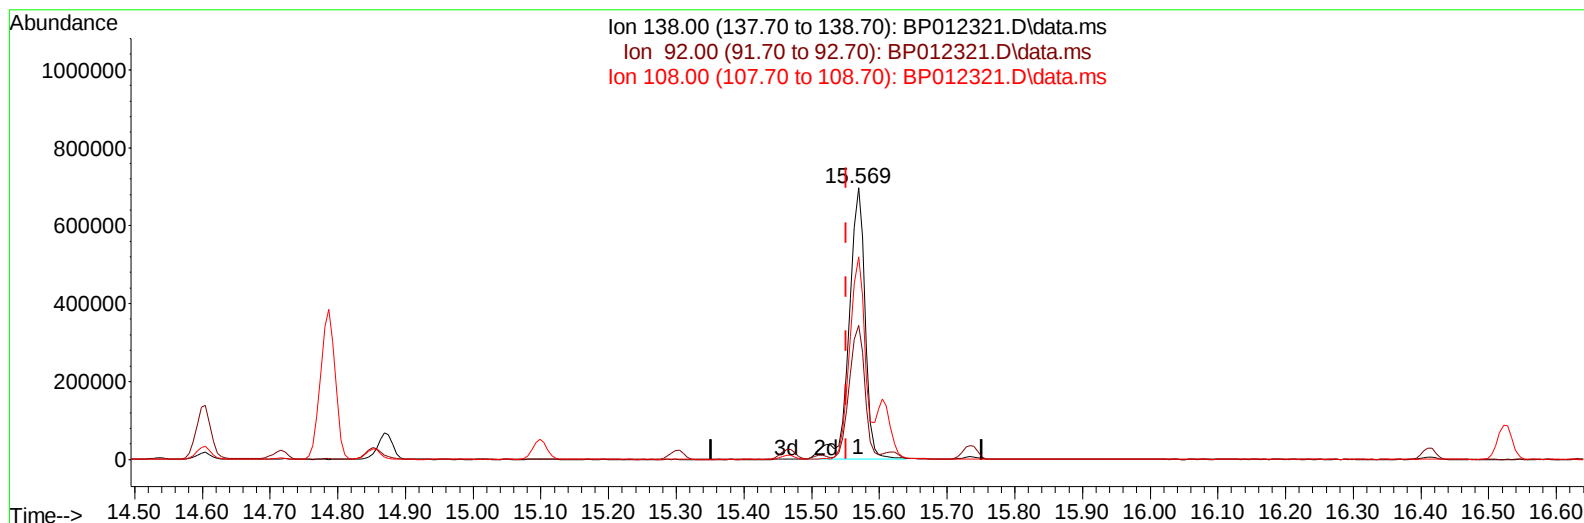

TIC: BP012321.D\data.ms

(63) 4-Nitroaniline

15.569min (+ 0.018) 81.58 ng/ul m

response 1147339

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	50.60	49.44
108.00	71.30	74.58
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102522\
 Data File : BP012321.D
 Acq On : 25 Oct 2022 18:45
 Operator : CG/JU
 Sample : SSTD08090
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD080607

Manual IntegrationsAPPROVED

Quant Time: Oct 27 03:10:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/27/2022
 Supervised By :mohammad ahmed 10/27/2022

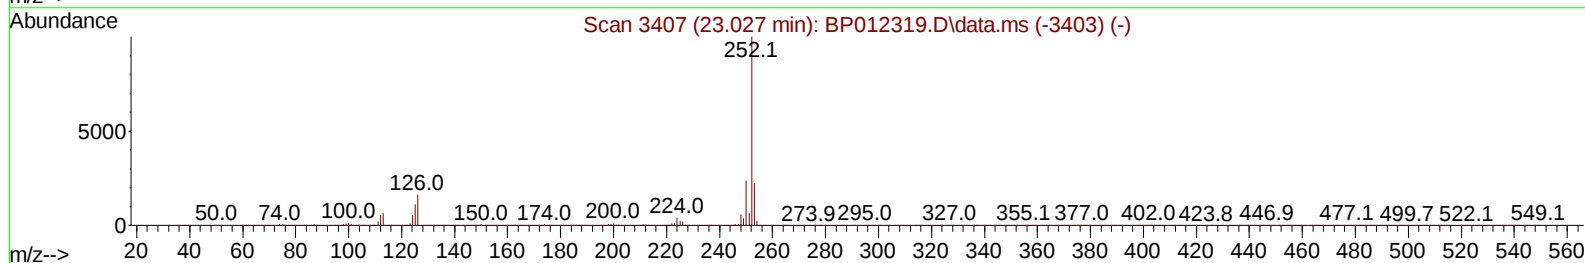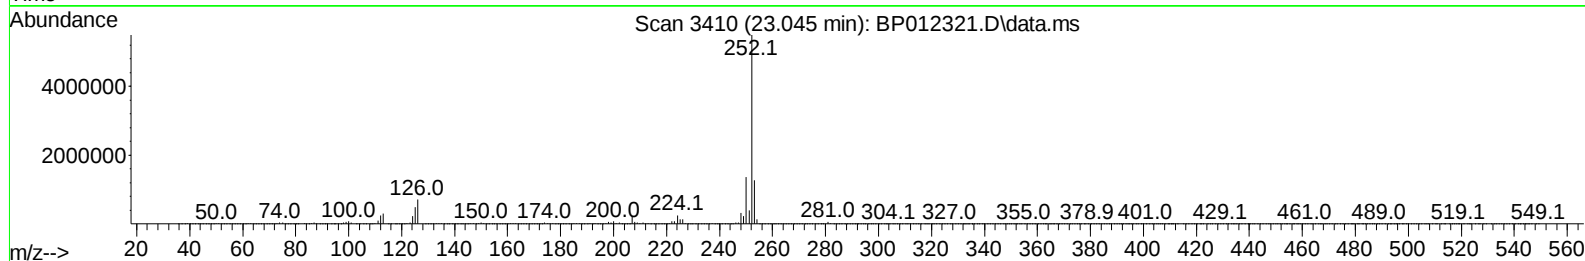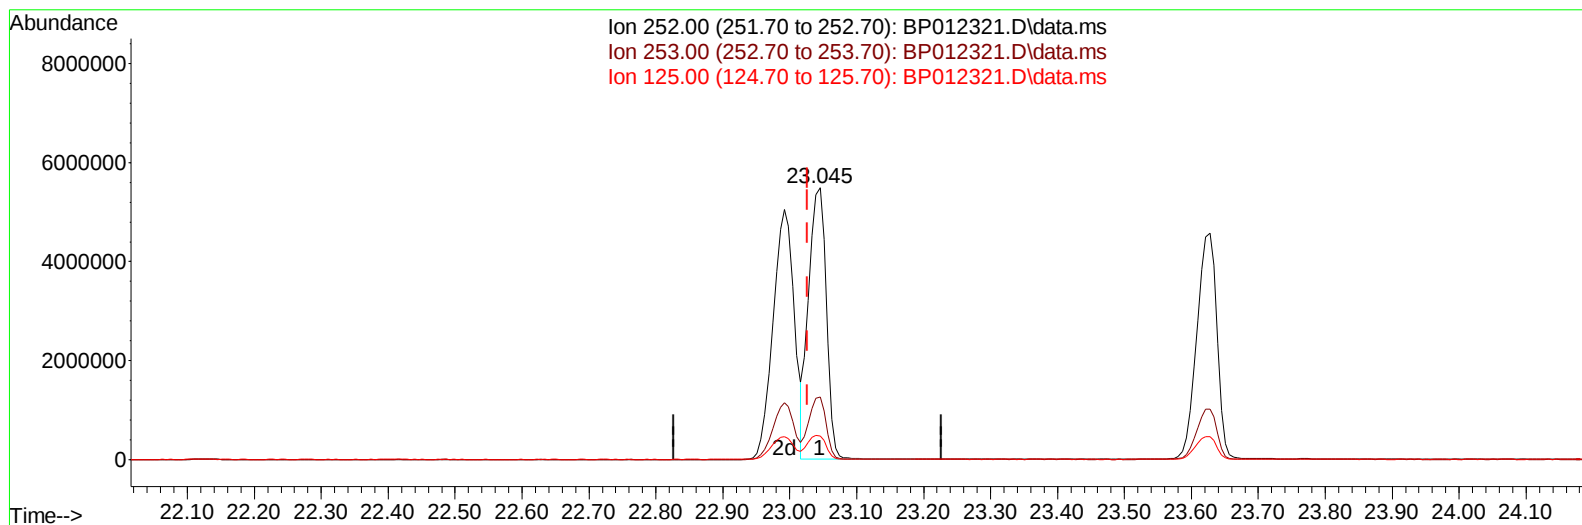

TIC: BP012321.D\data.ms

(91) Benzo(k)fluoranthene

23.045min (+ 0.018) 71.96 ng/u1

response 10116888

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.50	22.94
125.00	10.90	8.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102522\
 Data File : BP012321.D
 Acq On : 25 Oct 2022 18:45
 Operator : CG/JU
 Sample : SSTD08090
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD080607

Manual IntegrationsAPPROVED

Quant Time: Oct 26 10:08:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 10:05:01 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/27/2022
 Supervised By :mohammad ahmed 10/27/2022

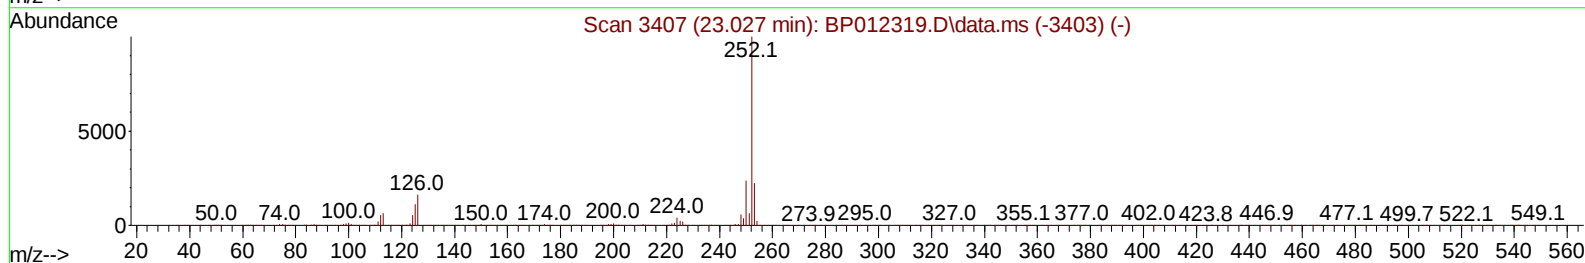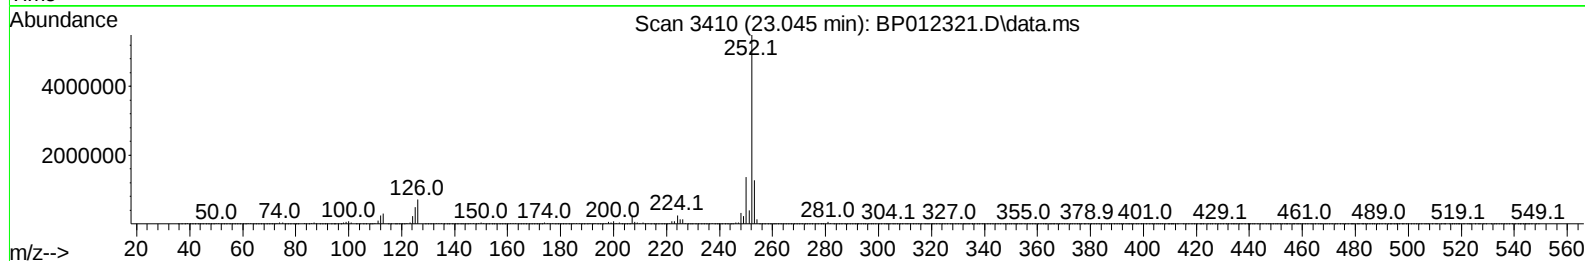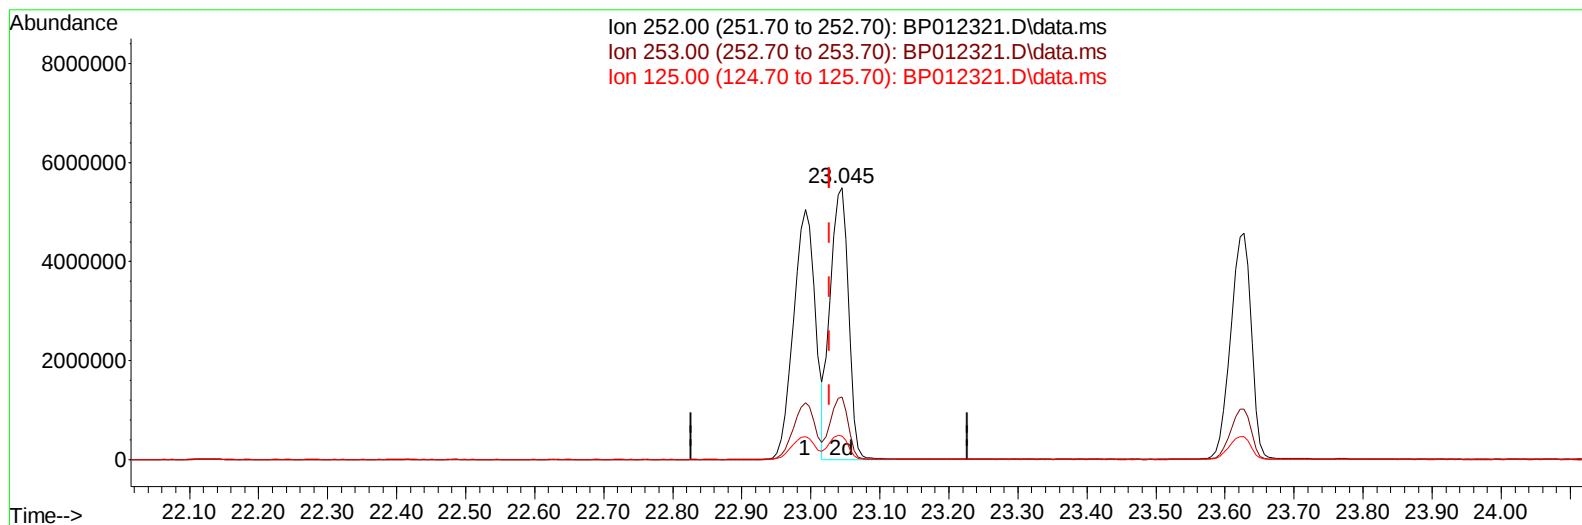

TIC: BP012321.D\data.ms

(91) Benzo(k)fluoranthene

23.045min (+ 0.018) 68.00 ng/ul m

response 10125655

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.20	22.94
125.00	11.20	8.72#
0.00	0.00	0.00