




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022631.D
Acq On : 26 Oct 2024 05:30
Operator : RC/JU
Sample : PB164386BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK386

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/26/2024
Supervised By :mohammad ahmed 10/29/2024

Quant Time: Oct 26 05:57:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 26 05:55:04 2024
Response via : Initial Calibration

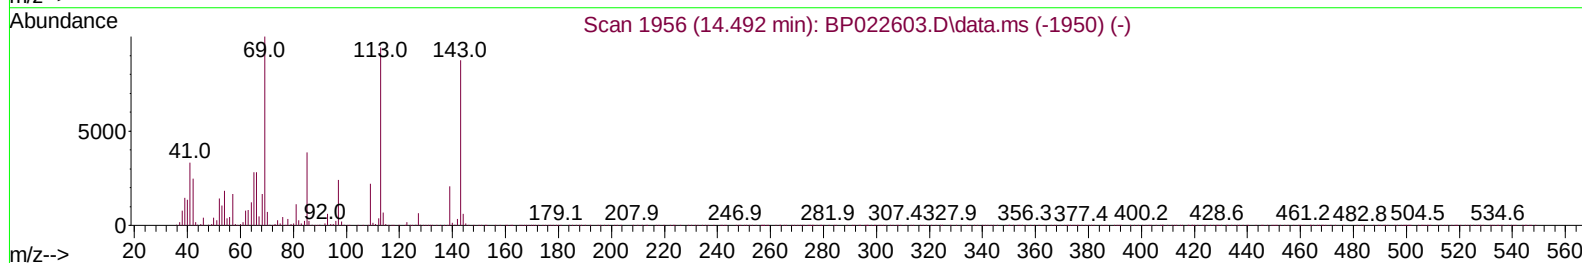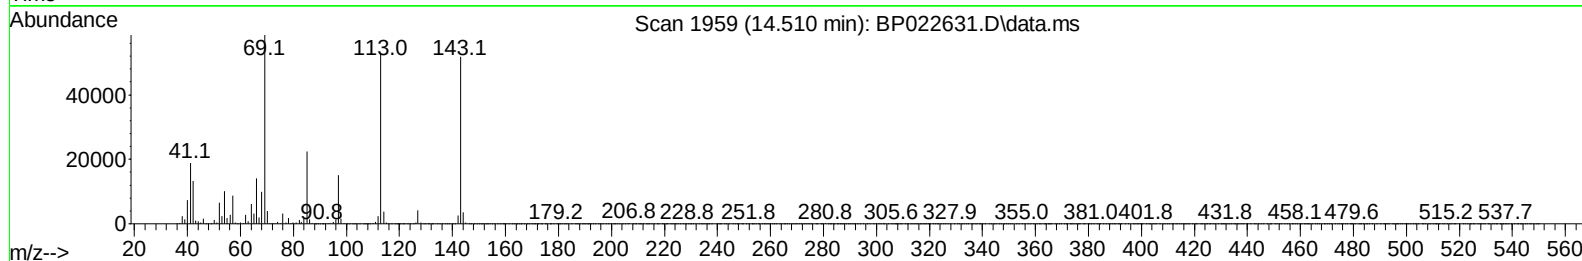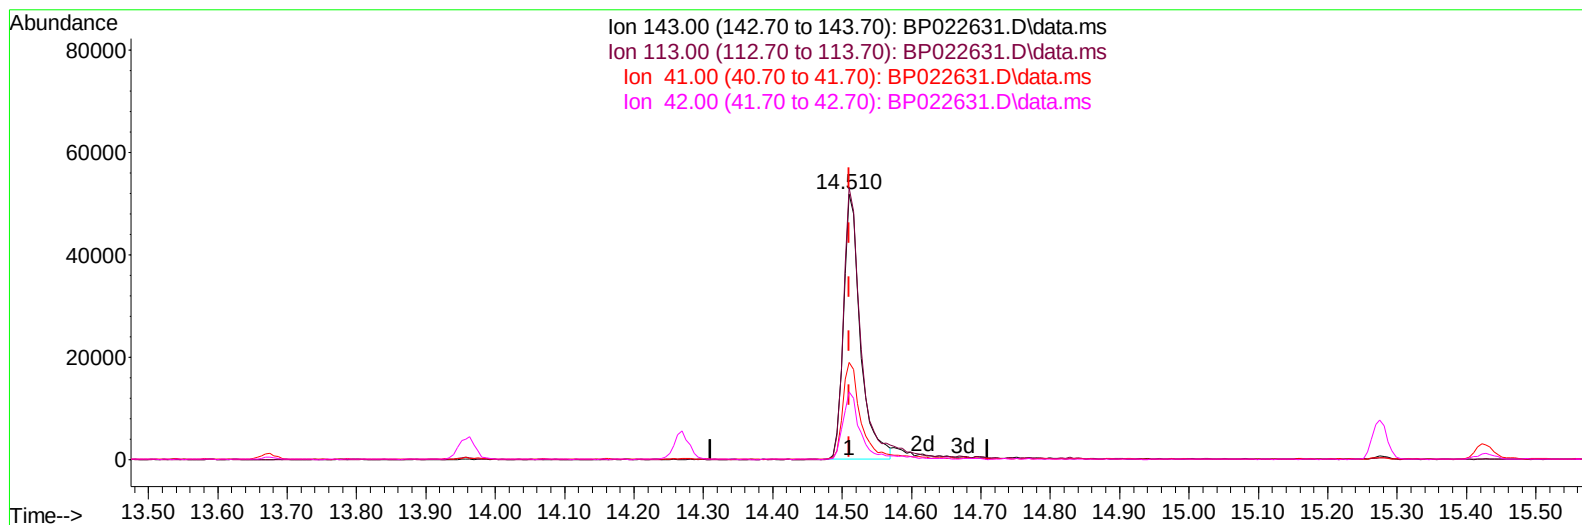

TIC: BP022631.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.510min (+ 0.000) 21.16 ng/ul

response 87936

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	102.27
41.00	35.90	36.52
42.00	23.70	25.56




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022631.D
Acq On : 26 Oct 2024 05:30
Operator : RC/JU
Sample : PB164386BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK386

Manual IntegrationsAPPROVED

Quant Time: Oct 26 05:57:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 26 05:55:04 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/26/2024
Supervised By :mohammad ahmed 10/29/2024

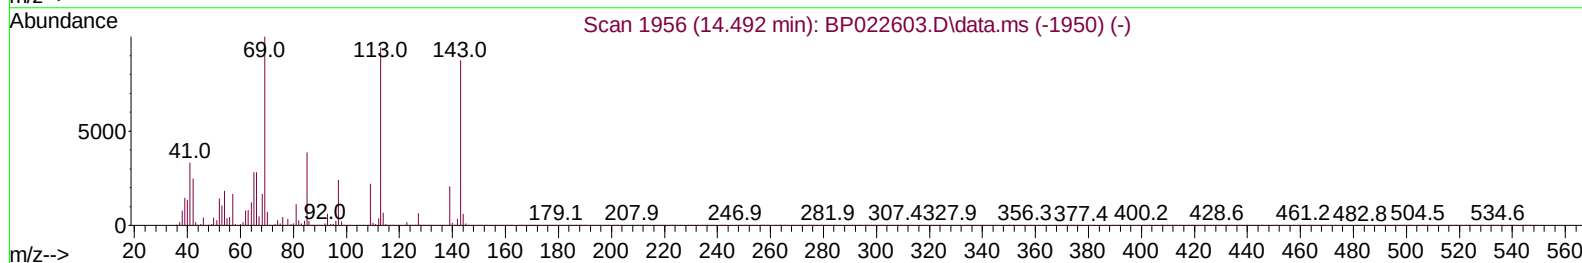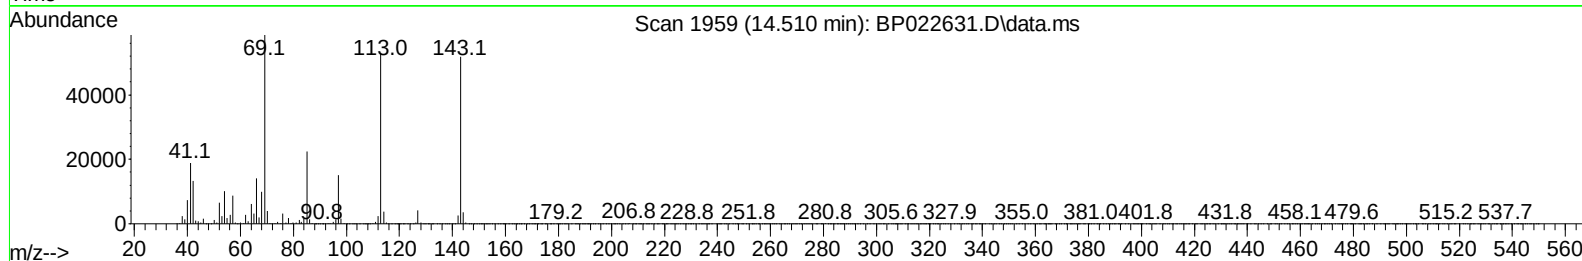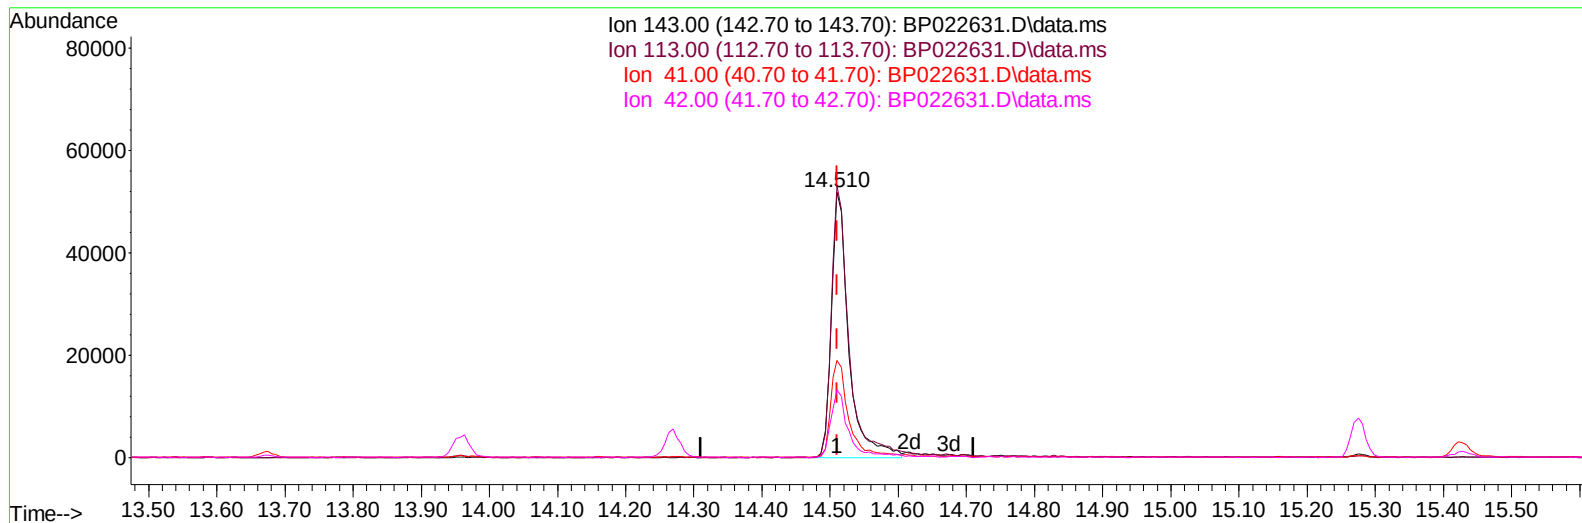

TIC: BP022631.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.510min (+ 0.000) 22.00 ng/ul m

response 91437

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	102.27
41.00	35.90	36.52
42.00	23.70	25.56

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022631.D
 Acq On : 26 Oct 2024 05:30
 Operator : RC/JU
 Sample : PB164386BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK386

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/26/2024
 Supervised By :mohammad ahmed 10/29/2024

Quant Time: Oct 26 06:04:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 26 05:55:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.652	152	103051	20.000	ng/ul	0.00
20) Naphthalene-d8	10.405	136	395961	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	311802	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.069	188	760412	20.000	ng/ul	0.00
79) Chrysene-d12	21.510	240	864720	20.000	ng/ul	0.00
88) Perylene-d12	24.774	264	960291	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	11873	4.477	ng/uL	0.00
4) Pyridine-d5	3.599	84	164135	22.546	ng/ul	0.00
7) Phenol-d5	6.840	99	211104	24.336	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	120743	23.683	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	161164	26.183	ng/ul	0.00
15) 4-Methylphenol-d8	8.358	113	172316	24.891	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	79645	26.160	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	95987	27.232	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	191559	25.570	ng/ul	0.00
31) 4-Chloroaniline-d4	10.546	131	222984	25.190	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	621948	25.106	ng/ul	0.00
49) Acenaphthylene-d8	13.963	160	672994	25.577	ng/ul	0.00
54) 4-Nitrophenol-d4	14.510	143	91437m	22.001	ng/ul	0.00
60) Fluorene-d10	15.275	176	551048	25.645	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.428	200	91201	18.236	ng/ul	0.01
73) Anthracene-d10	17.187	188	937520	26.208	ng/ul	0.02
81) Pyrene-d10	19.563	212	1194022	26.111	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.545	264	1376623	26.843	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022631.D
Acq On : 26 Oct 2024 05:30
Operator : RC/JU
Sample : PB164386BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK386

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/26/2024
Supervised By :mohammad ahmed 10/29/2024

Quant Time: Oct 26 06:04:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 26 05:55:04 2024
Response via : Initial Calibration

