

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022652.D
 Acq On : 26 Oct 2024 21:24
 Operator : RC/JU
 Sample : P4559-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNW6

Quant Time: Oct 28 00:30:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 26 05:55:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	66319	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.404	136	258360	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.263	164	203443	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.051	188	513050	20.000	ng/u1	-0.03
79) Chrysene-d12	21.486	240	615360	20.000	ng/u1	-0.01
88) Perylene-d12	24.745	264	730448	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	8760	5.133	ng/uL	-0.01
4) Pyridine-d5	3.605	84	29948	6.392	ng/u1	0.00
7) Phenol-d5	6.846	99	48719	8.727	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	109313	33.316	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.193	132	124520	31.435	ng/u1	-0.01
15) 4-Methylphenol-d8	8.352	113	98934	22.207	ng/u1	-0.01
21) Nitrobenzene-d5	8.787	128	72319	36.405	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.499	143	86560	37.637	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.046	165	174739	35.748	ng/u1	0.00
31) 4-Chloroaniline-d4	10.540	131	129340	22.393	ng/u1	-0.02
46) Dimethylphthalate-d6	13.663	166	615287	38.065	ng/u1	-0.02
49) Acenaphthylene-d8	13.951	160	620186	36.124	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.522	143	18841	6.948	ng/u1	0.02
60) Fluorene-d10	15.269	176	533504	38.053	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.398	200	106151	31.459	ng/u1	-0.02
73) Anthracene-d10	17.163	188	948110	39.283	ng/u1	0.00
81) Pyrene-d10	19.539	212	1264990	38.873	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.521	264	1610015	41.272	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.222	88	7519	4.098	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022652.D
Acq On : 26 Oct 2024 21:24
Operator : RC/JU
Sample : P4559-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNW6


Quant Time: Oct 28 00:30:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 26 05:55:04 2024
Response via : Initial Calibration

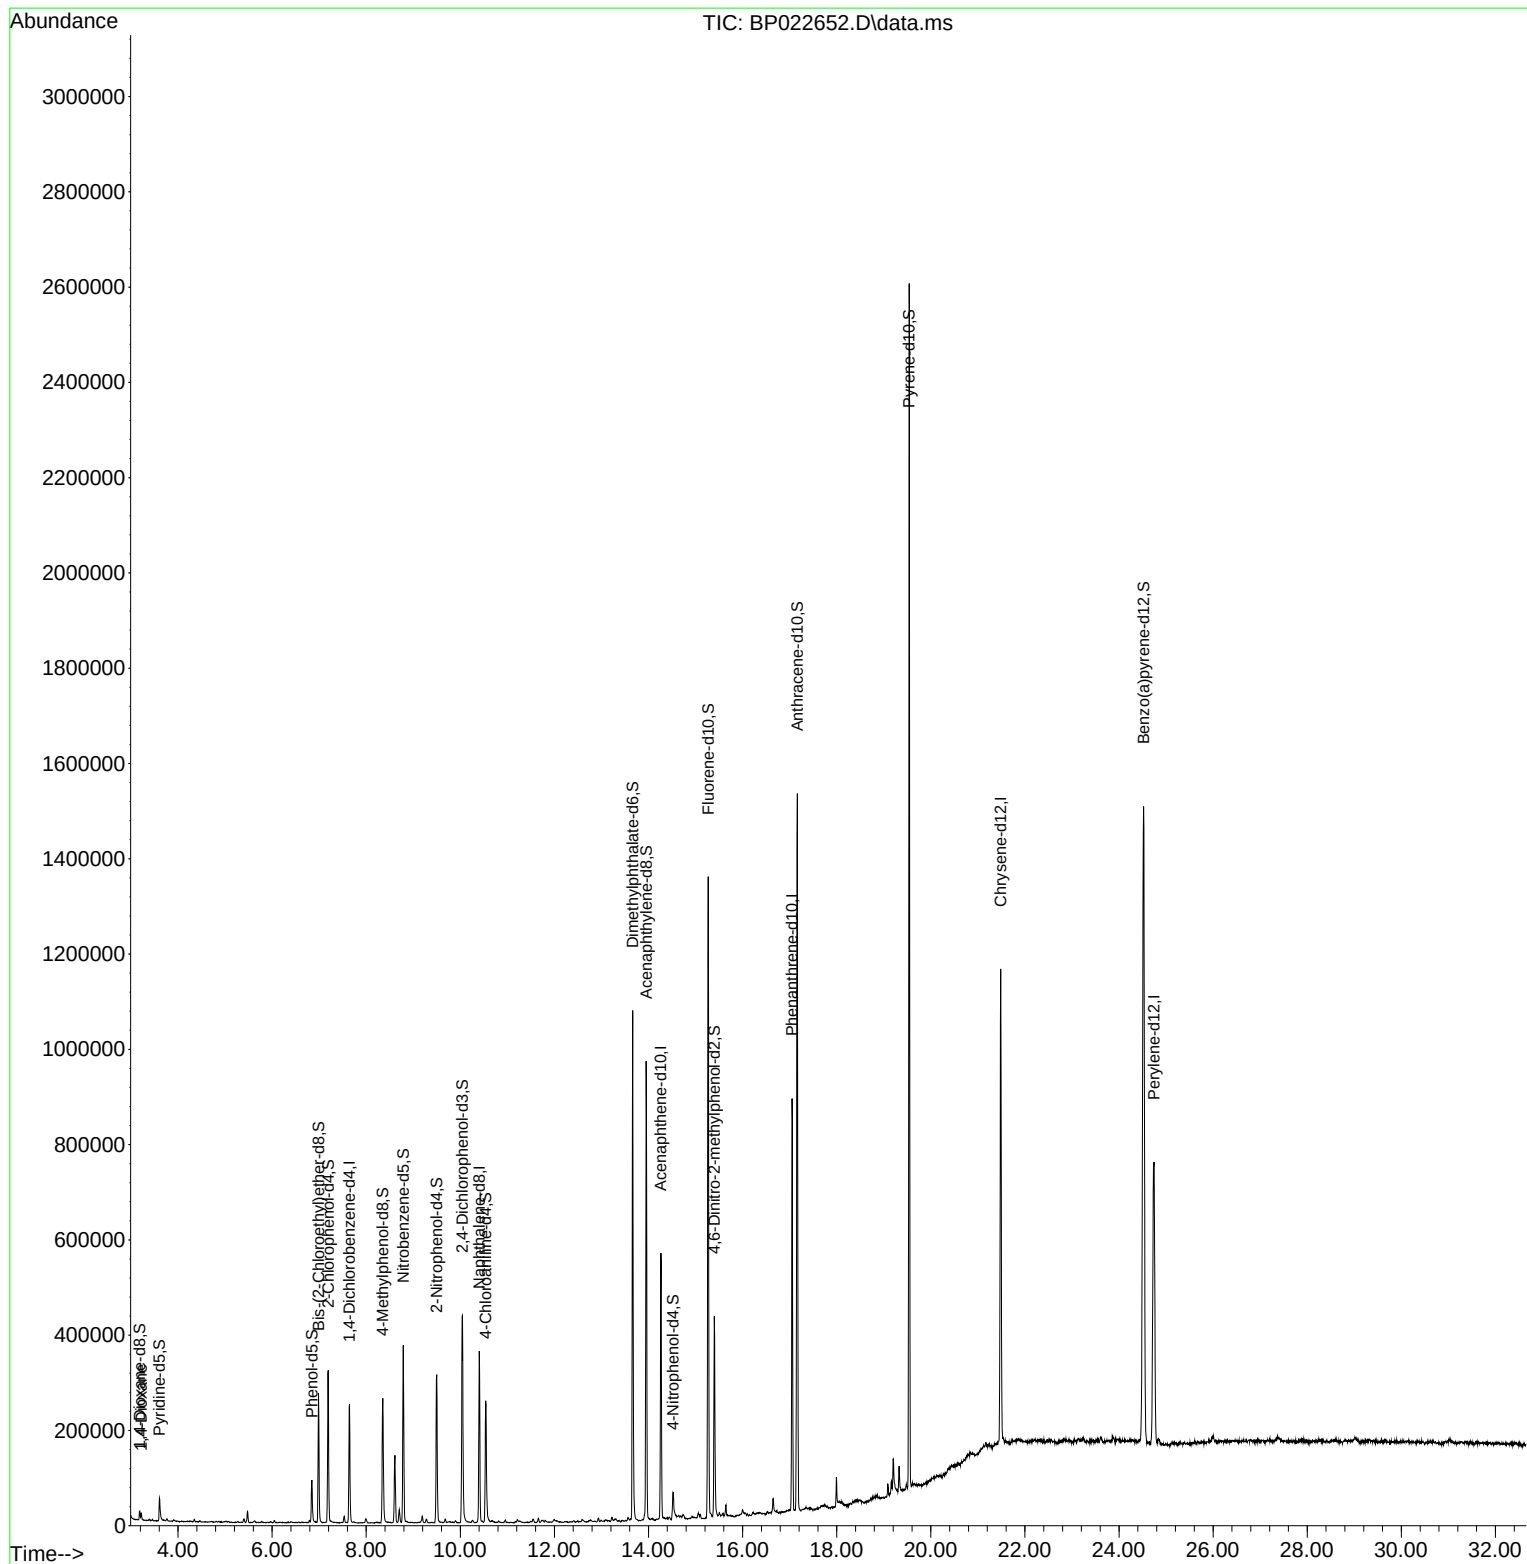

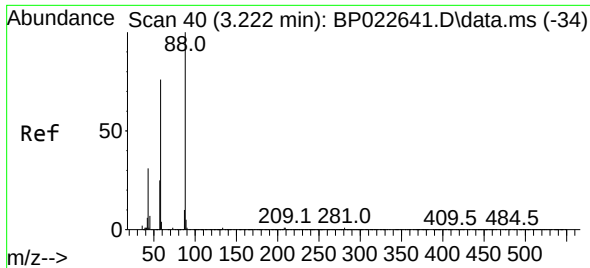

#2
 1,4-Dioxane
 Concen: 4.098 ng/uL
 RT: 3.222 min Scan# 40
 Delta R.T. -0.012 min
 Lab File: BP022652.D
 Acq: 26 Oct 2024 21:24

Instrument :
 BNA_P
 ClientSampleId :
 GCNW6

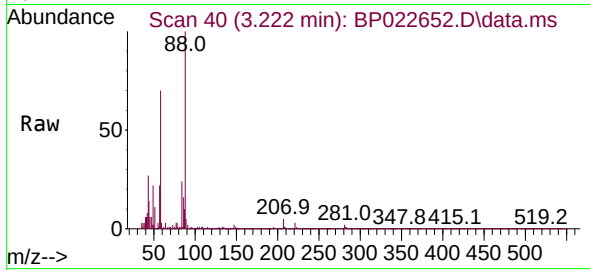

Tgt Ion:	88	Resp:	7519
Ion	Ratio	Lower	Upper
88	100		
43	26.9	22.3	33.5
58	70.1	54.7	82.1

