

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022619.D
 Acq On : 25 Oct 2024 20:40
 Operator : RC/JU
 Sample : PB164359BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK359

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	38	rBV	20932	25022	0.94%	0.096%
2	3.599	100	104	123	rBV	271452	418625	15.74%	1.612%
3	3.911	153	157	164	rVB	9386	12837	0.48%	0.049%
4	6.793	640	647	649	rBV3	4294	6270	0.24%	0.024%
5	6.840	649	655	669	rVB	331980	562921	21.16%	2.167%
6	6.993	674	681	694	rVB	259249	402418	15.13%	1.549%
7	7.193	708	715	727	rBV	346289	563345	21.18%	2.169%
8	7.652	785	793	803	rBV	347862	586912	22.06%	2.259%
9	8.357	905	913	930	rBV	386693	705865	26.53%	2.717%
10	8.793	979	987	1000	rBV	331729	559131	21.02%	2.152%
11	9.193	1048	1055	1063	rVB6	4976	8834	0.33%	0.034%
12	9.499	1095	1107	1118	rBV	280468	499583	18.78%	1.923%
13	10.046	1192	1200	1220	rBV	405027	770771	28.97%	2.967%
14	10.410	1253	1262	1273	rBV	524101	808389	30.39%	3.112%
15	10.546	1277	1285	1298	rBV	405983	708733	26.64%	2.728%
16	10.634	1298	1300	1307	rVV7	3568	6716	0.25%	0.026%
17	11.675	1473	1477	1481	rBV4	3400	5525	0.21%	0.021%
18	12.010	1527	1534	1543	rBV3	5945	13470	0.51%	0.052%
19	13.240	1737	1743	1747	rBV9	1335	2815	0.11%	0.011%
20	13.681	1811	1818	1826	rBV	823682	1185292	44.56%	4.563%
21	13.963	1855	1866	1878	rBV	877757	1326794	49.87%	5.108%
22	14.269	1910	1918	1927	rBV	799161	1189709	44.72%	4.580%
23	14.504	1952	1958	1968	rBV	284062	516471	19.41%	1.988%
24	15.275	2082	2089	2104	rBV	1098297	1737962	65.33%	6.691%
25	15.422	2106	2114	2128	rBV	336117	554732	20.85%	2.136%
26	15.516	2128	2130	2139	rVB7	7833	12092	0.45%	0.047%
27	16.081	2221	2226	2228	rBV6	1848	2954	0.11%	0.011%
28	16.745	2335	2339	2344	rBV6	2288	3198	0.12%	0.012%
29	16.857	2354	2358	2360	rBV5	2266	3360	0.13%	0.013%
30	17.069	2388	2394	2405	rBV	1025336	1553893	58.41%	5.982%
31	17.175	2405	2412	2425	rVV2	1278440	1969164	74.02%	7.581%
32	18.016	2550	2555	2558	rBV6	5798	10057	0.38%	0.039%
33	18.516	2638	2640	2645	rBV6	2983	4473	0.17%	0.017%
34	19.110	2737	2741	2745	rVB3	20468	27269	1.03%	0.105%
35	19.180	2748	2753	2757	rBV	22257	32331	1.22%	0.124%
36	19.557	2811	2817	2826	rBV	1853730	2549514	95.84%	9.815%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022619.D
Acq On : 25 Oct 2024 20:40
Operator : RC/JU
Sample : PB164359BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK359

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	21.510	3143	3149	3160	rVB2	1215228	1965181	73.87%	7.565%
38	24.551	3657	3666	3676	rVB	985476	2660288	100.00%	10.241%
39	24.780	3695	3705	3718	rVB	735915	2003353	75.31%	7.712%


Sum of corrected areas: 25976269

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022619.D
Acq On : 25 Oct 2024 20:40
Operator : RC/JU
Sample : PB164359BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK359

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

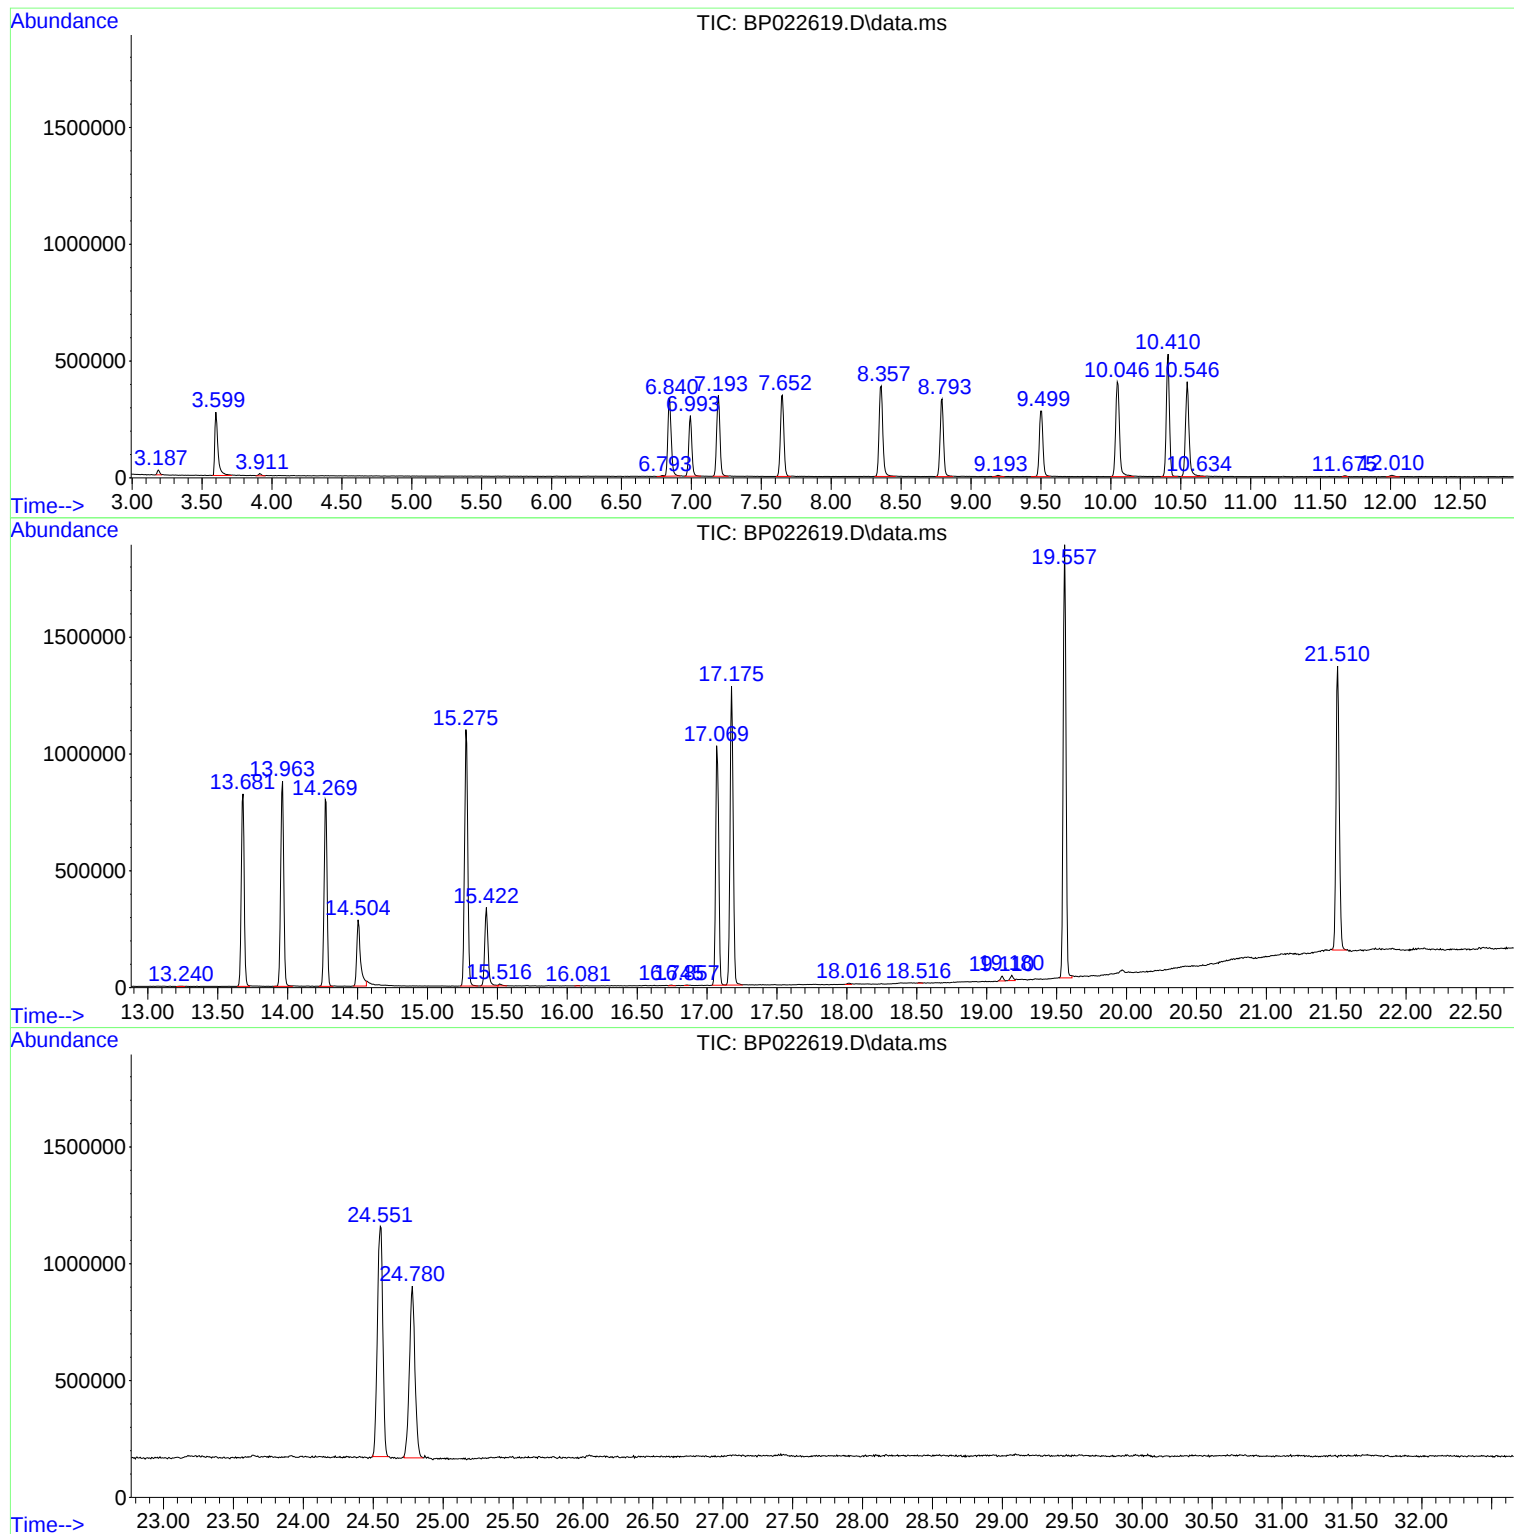

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022619.D
Acq On : 25 Oct 2024 20:40
Operator : RC/JU
Sample : PB164359BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK359

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022619.D
Acq On : 25 Oct 2024 20:40
Operator : RC/JU
Sample : PB164359BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK359

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc