

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022631.D
 Acq On : 26 Oct 2024 05:30
 Operator : RC/JU
 Sample : PB164386BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK386

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	40	rBV	23348	30803	0.99%	0.104%
2	3.599	100	104	122	rBV	297469	456226	14.73%	1.546%
3	3.911	152	157	163	rVB	5189	7975	0.26%	0.027%
4	6.840	649	655	666	rBV	362572	619964	20.02%	2.100%
5	6.993	673	681	694	rVB	283434	442550	14.29%	1.499%
6	7.193	708	715	733	rBV	391201	627376	20.26%	2.126%
7	7.652	784	793	806	rBV	379268	623399	20.13%	2.112%
8	8.358	905	913	928	rBV	481066	802795	25.92%	2.720%
9	8.793	979	987	998	rBV	378222	626885	20.24%	2.124%
10	9.199	1049	1056	1061	rVB8	3648	5966	0.19%	0.020%
11	9.505	1100	1108	1121	rBV	318958	565803	18.27%	1.917%
12	10.046	1192	1200	1216	rBV	478389	882764	28.50%	2.991%
13	10.405	1253	1261	1270	rBV	484770	859622	27.75%	2.912%
14	10.546	1278	1285	1304	rBV	475894	812340	26.23%	2.752%
15	11.675	1470	1477	1484	rBV10	1893	3148	0.10%	0.011%
16	11.999	1524	1532	1539	rBV2	6779	14955	0.48%	0.051%
17	13.675	1810	1817	1830	rBV	877892	1328354	42.89%	4.501%
18	13.963	1858	1866	1878	rBV	923750	1536554	49.61%	5.206%
19	14.269	1909	1918	1931	rVB	841607	1325580	42.80%	4.491%
20	14.510	1953	1959	1980	rBV	361757	661876	21.37%	2.242%
21	15.275	2083	2089	2099	rBV	1336703	1992806	64.34%	6.752%
22	15.428	2107	2115	2128	rBV	306131	548783	17.72%	1.859%
23	15.528	2128	2132	2137	rVB2	9170	14285	0.46%	0.048%
24	16.081	2220	2226	2229	rBV8	2357	3230	0.10%	0.011%
25	16.869	2355	2360	2365	rBV6	2749	5423	0.18%	0.018%
26	17.069	2386	2394	2406	rBV	1076191	1776588	57.36%	6.019%
27	17.187	2406	2414	2424	rBV	1565119	2314912	74.74%	7.843%
28	17.381	2443	2447	2451	rBV6	1921	3158	0.10%	0.011%
29	17.492	2463	2466	2470	rBV6	2691	3855	0.12%	0.013%
30	18.016	2551	2555	2557	rVV5	3421	4582	0.15%	0.016%
31	19.098	2735	2739	2744	rBV2	21086	29513	0.95%	0.100%
32	19.186	2748	2754	2759	rBV3	20153	40930	1.32%	0.139%
33	19.563	2811	2818	2829	rVB	1942908	2914913	94.11%	9.876%
34	21.510	3143	3149	3157	rBV	1573614	2260421	72.98%	7.658%
35	24.545	3656	3665	3675	rVB	1298179	3097263	100.00%	10.494%
36	24.774	3694	3704	3714	rVB	820259	2269743	73.28%	7.690%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022631.D
Acq On : 26 Oct 2024 05:30
Operator : RC/JU
Sample : PB164386BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK386

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 29515340

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022631.D
Acq On : 26 Oct 2024 05:30
Operator : RC/JU
Sample : PB164386BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK386

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

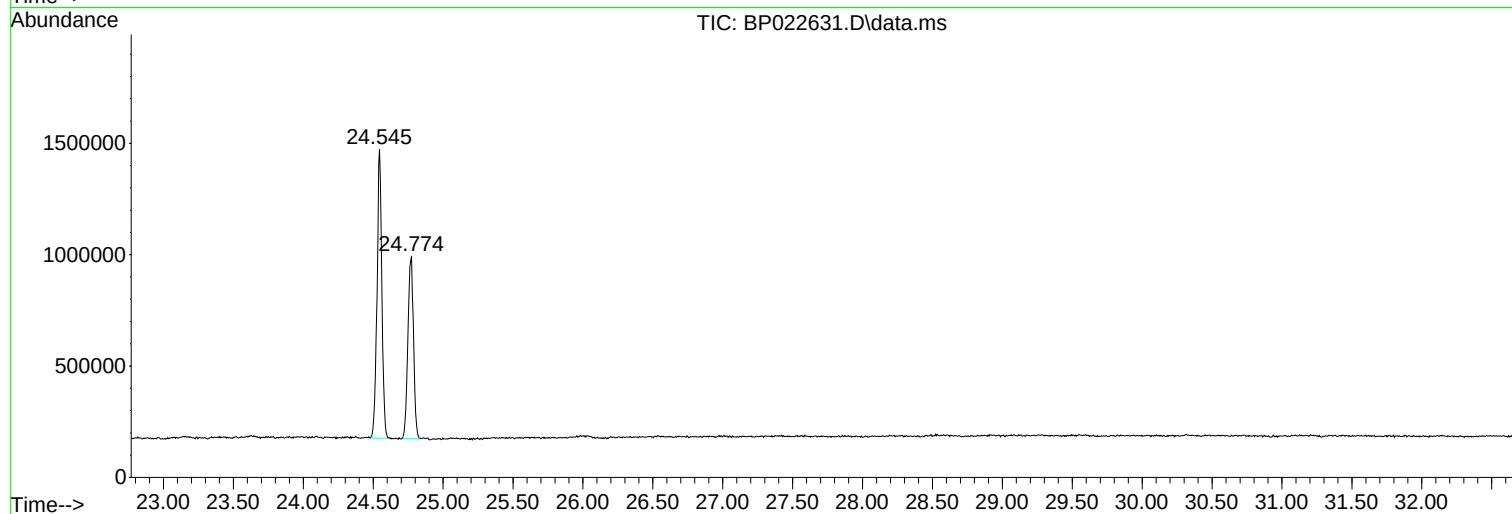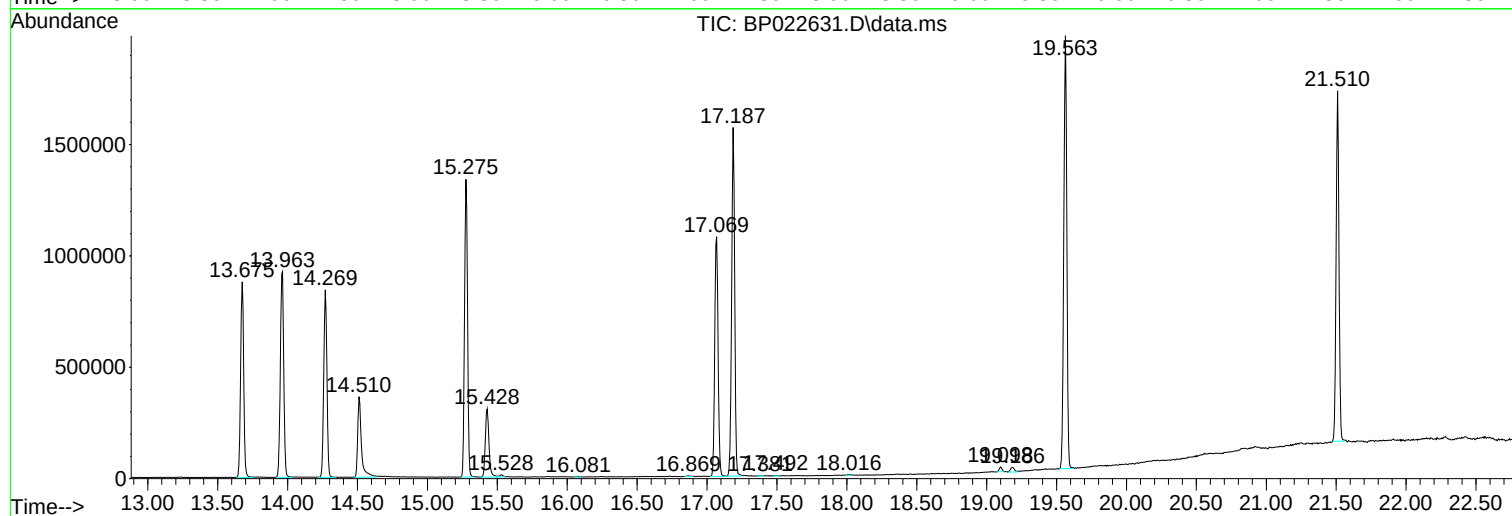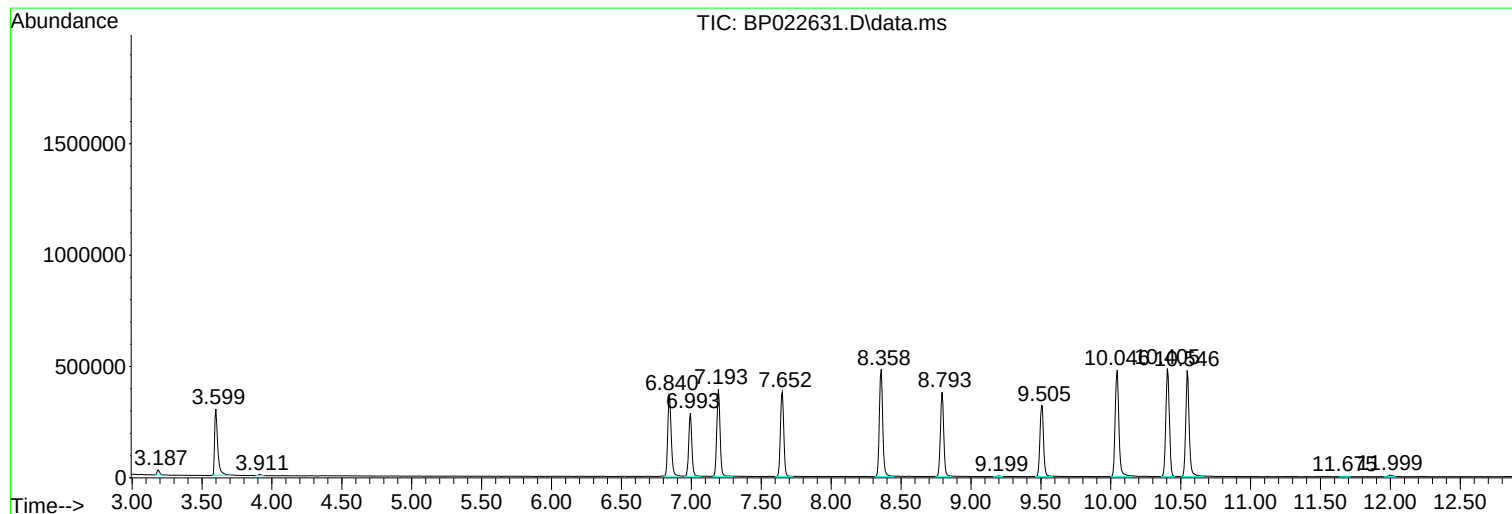

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022631.D
Acq On : 26 Oct 2024 05:30
Operator : RC/JU
Sample : PB164386BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK386

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022631.D
Acq On : 26 Oct 2024 05:30
Operator : RC/JU
Sample : PB164386BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK386

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc