

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022637.D
 Acq On : 26 Oct 2024 11:17
 Operator : RC/JU
 Sample : P4532-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	39	rBV	17065	21672	0.59%	0.071%
2	3.605	101	105	114	rBV	80754	128903	3.49%	0.423%
3	3.917	154	158	164	rVB	5546	8995	0.24%	0.029%
4	4.287	217	221	227	rVB9	4668	7638	0.21%	0.025%
5	4.458	247	250	254	rBV5	2674	4129	0.11%	0.014%
6	5.499	421	427	438	rVB4	8364	15217	0.41%	0.050%
7	5.711	459	463	468	rVB8	3128	5552	0.15%	0.018%
8	6.028	511	517	521	rBV2	23394	37224	1.01%	0.122%
9	6.264	550	557	570	rVB9	5625	18969	0.51%	0.062%
10	6.475	587	593	597	rVV2	11083	18016	0.49%	0.059%
11	6.522	597	601	608	rVB	15394	22114	0.60%	0.072%
12	6.705	627	632	639	rBV8	3468	7008	0.19%	0.023%
13	6.846	650	656	668	rVB2	98373	174277	4.72%	0.571%
14	6.993	673	681	690	rBV	312001	480994	13.03%	1.577%
15	7.193	707	715	726	rBV	367951	609236	16.50%	1.997%
16	7.269	726	728	734	rVB7	2710	3927	0.11%	0.013%
17	7.646	783	792	801	rBV	362360	590205	15.99%	1.935%
18	8.358	905	913	927	rBV	310495	537242	14.55%	1.761%
19	8.787	978	986	1003	rBV	406434	697351	18.89%	2.286%
20	8.928	1005	1010	1021	rVB4	6382	13495	0.37%	0.044%
21	9.193	1050	1055	1061	rVB3	5448	8776	0.24%	0.029%
22	9.505	1101	1108	1121	rBV	359040	630891	17.09%	2.068%
23	9.722	1139	1145	1148	rBV4	4228	9681	0.26%	0.032%
24	9.769	1151	1153	1161	rVB7	4390	6508	0.18%	0.021%
25	10.046	1192	1200	1215	rBV	517379	964466	26.13%	3.162%
26	10.405	1250	1261	1269	rBV	486205	815200	22.08%	2.672%
27	10.546	1278	1285	1300	rBV	361170	677919	18.36%	2.222%
28	11.222	1391	1400	1412	rBV8	7888	21864	0.59%	0.072%
29	11.669	1472	1476	1482	rVB4	4825	7306	0.20%	0.024%
30	11.993	1526	1531	1539	rBV3	9757	16264	0.44%	0.053%
31	13.669	1809	1816	1829	rBV	1068991	1511168	40.94%	4.954%
32	13.951	1856	1864	1879	rBV	1133896	1689539	45.77%	5.538%
33	14.263	1910	1917	1928	rBV	866220	1260680	34.15%	4.133%
34	14.516	1953	1960	1980	rBV2	67678	198538	5.38%	0.651%
35	14.698	1984	1991	1997	rVB2	3428	10287	0.28%	0.034%
36	15.281	2081	2090	2096	rBV	1664469	2263346	61.31%	7.419%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022637.D
 Acq On : 26 Oct 2024 11:17
 Operator : RC/JU
 Sample : P4532-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.328	2096	2098	2105	rVV6	11066	16249	0.44%	0.053%
38	15.404	2105	2111	2124	rVV	524363	746158	20.21%	2.446%
39	15.522	2127	2131	2137	rVB5	6594	11261	0.31%	0.037%
40	15.651	2148	2153	2157	rVB	21052	28466	0.77%	0.093%
41	15.851	2181	2187	2192	rBV10	2343	5095	0.14%	0.017%
42	16.004	2205	2213	2220	rBV	11420	22357	0.61%	0.073%
43	16.275	2255	2259	2263	rVB2	3318	4113	0.11%	0.013%
44	16.663	2320	2325	2329	rBV6	4830	7447	0.20%	0.024%
45	16.734	2331	2337	2341	rBV9	3116	5980	0.16%	0.020%
46	16.845	2350	2356	2363	rBV7	3606	6698	0.18%	0.022%
47	17.069	2388	2394	2403	rBV	1499895	1692494	45.85%	5.548%
48	17.163	2403	2410	2424	rVV	1926740	2756937	74.69%	9.037%
49	17.763	2508	2512	2517	rBV7	6851	8219	0.22%	0.027%
50	18.004	2549	2553	2562	rBV2	35737	55546	1.50%	0.182%
51	18.075	2562	2565	2568	rVB2	6522	7644	0.21%	0.025%
52	19.098	2735	2739	2747	rBV3	26863	40276	1.09%	0.132%
53	19.175	2748	2752	2755	rBV	28983	37827	1.02%	0.124%
54	19.216	2755	2759	2767	rVB4	39597	65049	1.76%	0.213%
55	19.345	2777	2781	2785	rBV4	45905	57843	1.57%	0.190%
56	19.551	2810	2816	2826	rBV	2419770	3477488	94.21%	11.399%
57	21.504	3142	3148	3158	rVB	1448105	2130582	57.72%	6.984%
58	24.545	3655	3665	3676	rVB	1580231	3691374	100.00%	12.101%
59	24.763	3694	3702	3713	rVB	793792	2136088	57.87%	7.002%




Sum of corrected areas: 30505788

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022637.D
Acq On : 26 Oct 2024 11:17
Operator : RC/JU
Sample : P4532-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

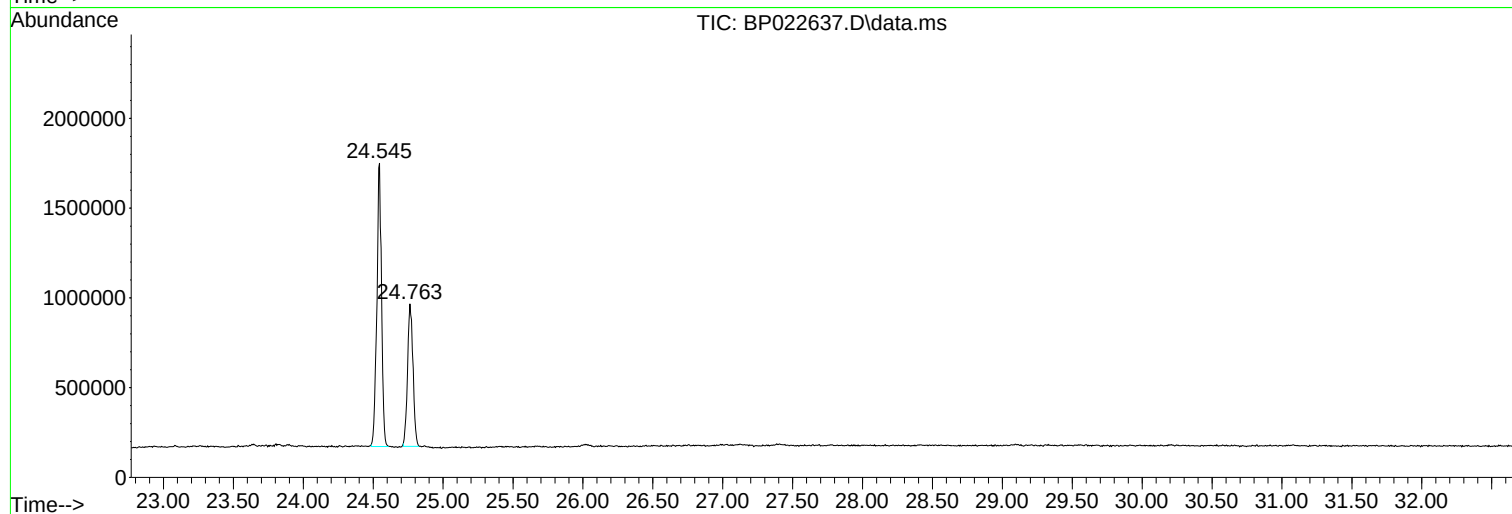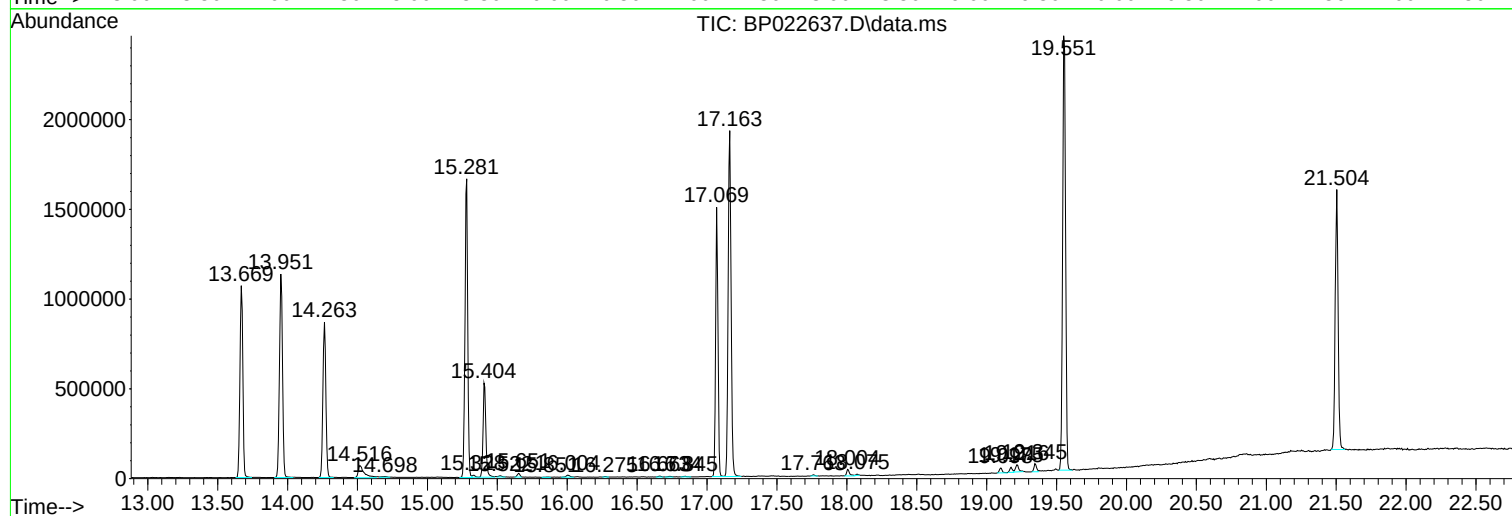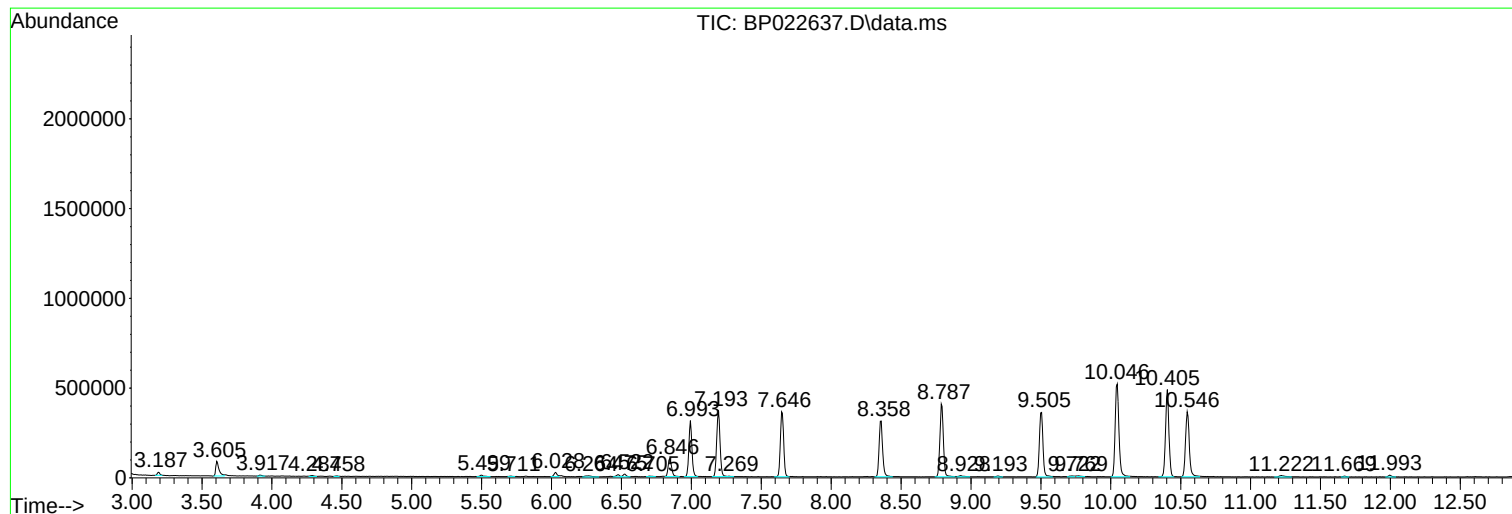

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022637.D
Acq On : 26 Oct 2024 11:17
Operator : RC/JU
Sample : P4532-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022637.D
Acq On : 26 Oct 2024 11:17
Operator : RC/JU
Sample : P4532-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc