

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022638.D
 Acq On : 26 Oct 2024 11:58
 Operator : RC/JU
 Sample : P4532-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.105	15	20	23	rBV6	2468	4616	0.12%	0.015%
2	3.187	30	34	39	rBV	18057	22862	0.61%	0.074%
3	3.605	102	105	115	rBV	53031	95275	2.52%	0.310%
4	3.911	153	157	163	rVB3	5508	8094	0.21%	0.026%
5	4.281	216	220	224	rBV6	3406	4802	0.13%	0.016%
6	5.493	422	426	438	rVB9	6876	13363	0.35%	0.043%
7	5.711	454	463	468	rBV9	2621	5061	0.13%	0.016%
8	6.028	511	517	522	rBV3	19069	33507	0.89%	0.109%
9	6.258	549	556	565	rVB3	4241	11231	0.30%	0.037%
10	6.475	589	593	597	rBV2	7990	12242	0.32%	0.040%
11	6.522	597	601	608	rVB2	13308	21475	0.57%	0.070%
12	6.711	629	633	641	rBV10	2141	5429	0.14%	0.018%
13	6.793	643	647	650	rVV5	2548	3787	0.10%	0.012%
14	6.846	650	656	669	rVB	101848	180012	4.76%	0.586%
15	6.993	674	681	692	rBV	310594	484236	12.82%	1.575%
16	7.193	708	715	726	rBV	370660	602495	15.95%	1.960%
17	7.652	785	793	801	rBV	363871	598616	15.84%	1.947%
18	8.352	905	912	931	rVV	320063	552134	14.61%	1.796%
19	8.787	978	986	995	rBV	394823	692597	18.33%	2.253%
20	9.193	1051	1055	1062	rVB5	4295	7956	0.21%	0.026%
21	9.504	1100	1108	1124	rBV	385990	643438	17.03%	2.093%
22	9.769	1148	1153	1158	rBV9	2571	4428	0.12%	0.014%
23	10.040	1190	1199	1219	rBV	536820	1008147	26.68%	3.280%
24	10.404	1253	1261	1272	rBV	496684	839832	22.23%	2.732%
25	10.546	1278	1285	1300	rBV	339117	633938	16.78%	2.062%
26	11.222	1393	1400	1408	rBV6	5187	11350	0.30%	0.037%
27	11.675	1474	1477	1484	rVB7	2706	4444	0.12%	0.014%
28	11.816	1493	1501	1507	rBV3	4798	10338	0.27%	0.034%
29	11.998	1525	1532	1542	rBV2	7765	15426	0.41%	0.050%
30	12.863	1673	1679	1685	rVB2	2325	5194	0.14%	0.017%
31	13.457	1774	1780	1783	rBV7	2575	4948	0.13%	0.016%
32	13.669	1808	1816	1825	rBV	1111738	1618498	42.84%	5.265%
33	13.951	1855	1864	1880	rBV	1188263	1749866	46.32%	5.692%
34	14.263	1910	1917	1927	rBV	824300	1227370	32.49%	3.993%
35	14.516	1953	1960	1967	rBV	86990	173710	4.60%	0.565%
36	14.581	1967	1971	1981	rVB3	20057	42273	1.12%	0.138%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022638.D
Acq On : 26 Oct 2024 11:58
Operator : RC/JU
Sample : P4532-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	14.704	1987	1992	2000	rVB10	6439	13064	0.35%	0.042%
38	15.045	2045	2050	2053	rBV7	1863	3939	0.10%	0.013%
39	15.269	2081	2088	2096	rBV	1571173	2353073	62.28%	7.655%
40	15.328	2096	2098	2105	rVV7	5561	8466	0.22%	0.028%
41	15.410	2106	2112	2126	rVV	538372	813220	21.53%	2.645%
42	15.510	2126	2129	2138	rVB5	9193	17104	0.45%	0.056%
43	15.645	2145	2152	2159	rBV	94107	135328	3.58%	0.440%
44	16.004	2206	2213	2219	rBV	11969	22755	0.60%	0.074%
45	16.216	2246	2249	2254	rVB3	5752	6229	0.16%	0.020%
46	16.734	2333	2337	2342	rVB7	2537	4331	0.11%	0.014%
47	16.834	2349	2354	2355	rBV5	4130	5964	0.16%	0.019%
48	17.063	2385	2393	2402	rBV	1087795	1629197	43.12%	5.300%
49	17.163	2403	2410	2422	rVV	1869626	2780724	73.60%	9.046%
50	17.469	2458	2462	2465	rBV5	3340	5567	0.15%	0.018%
51	17.986	2546	2550	2559	rBV2	60092	93945	2.49%	0.306%
52	18.063	2561	2563	2569	rVB2	7307	9739	0.26%	0.032%
53	19.080	2732	2736	2741	rBV3	25124	37074	0.98%	0.121%
54	19.157	2745	2749	2753	rBV	27751	42839	1.13%	0.139%
55	19.198	2753	2756	2766	rVB	94399	136768	3.62%	0.445%
56	19.328	2773	2778	2784	rBV3	43341	70247	1.86%	0.229%
57	19.539	2808	2814	2822	rBV	2607227	3490871	92.40%	11.356%
58	21.492	3140	3146	3153	rVB	1179681	1903288	50.38%	6.191%
59	24.539	3653	3664	3676	rVB	1362395	3777984	100.00%	12.290%
60	24.768	3694	3703	3713	rVB	731644	2025805	53.62%	6.590%




Sum of corrected areas: 30740511

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022638.D
Acq On : 26 Oct 2024 11:58
Operator : RC/JU
Sample : P4532-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

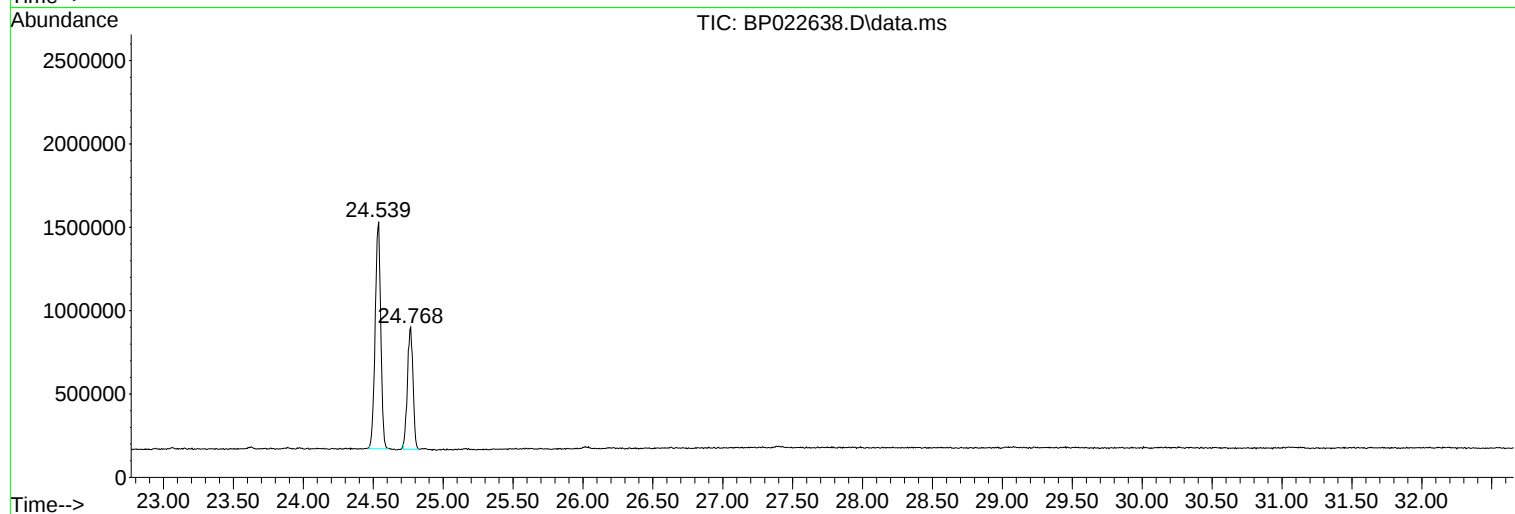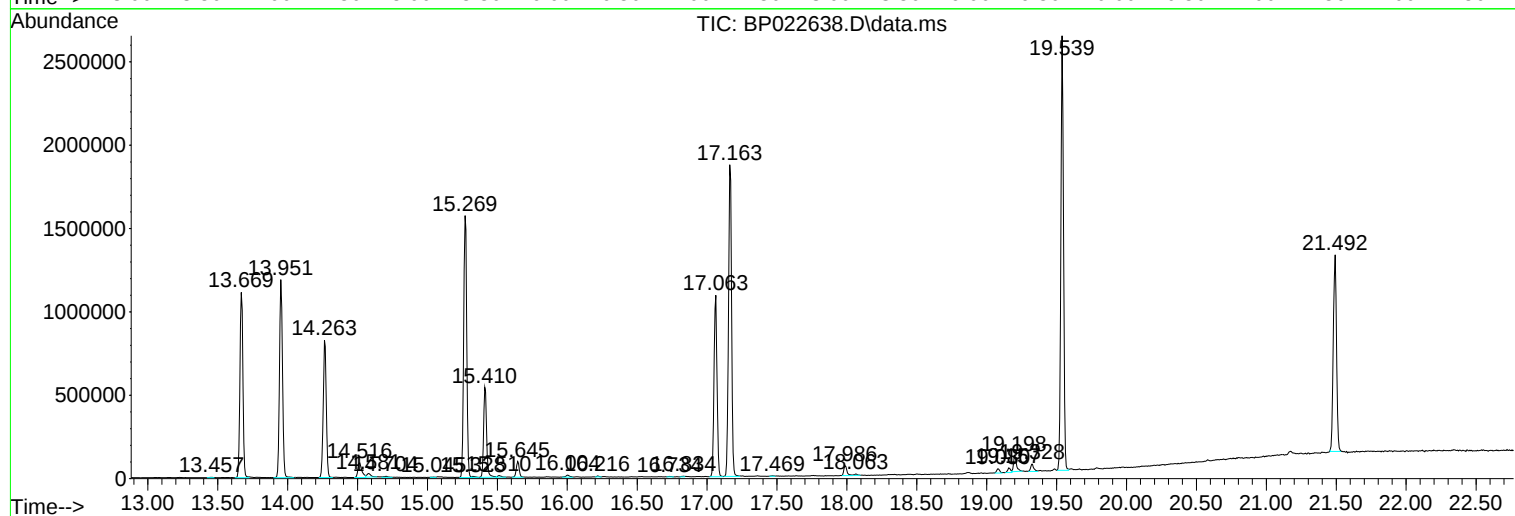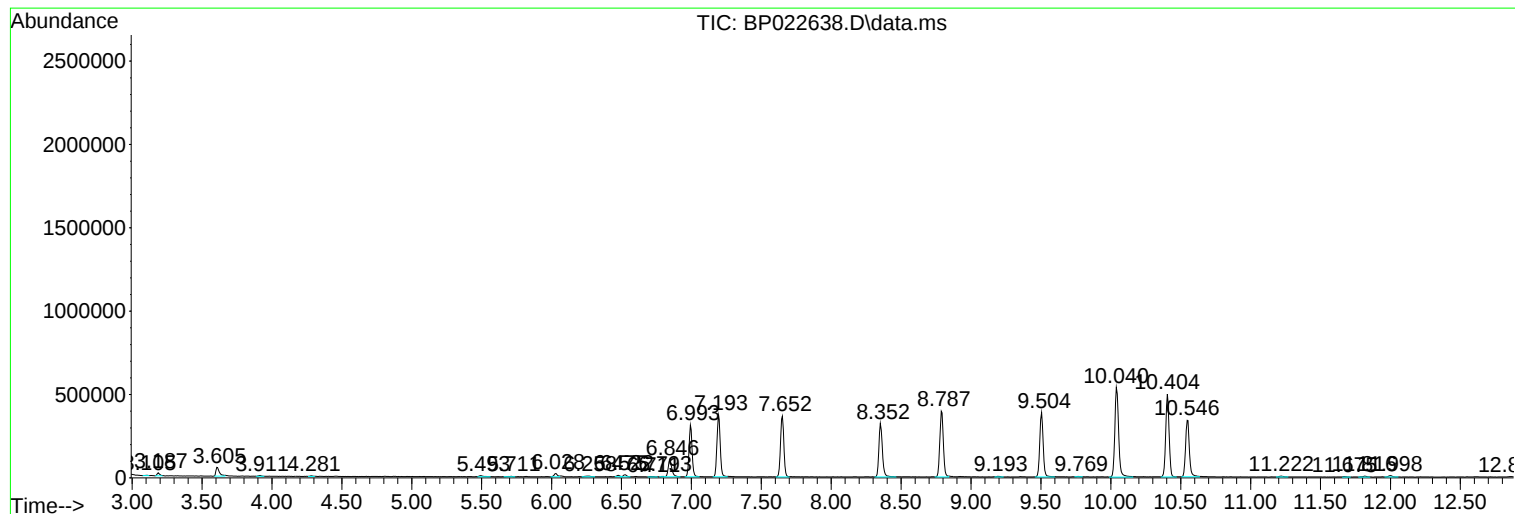

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022638.D
Acq On : 26 Oct 2024 11:58
Operator : RC/JU
Sample : P4532-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNW5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.645	2.21 ng/ul	135328	Acenaphthene-d10	14.263

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	95
3			Benzophenone	182	C13H10O	000119-61-9	91
4			Benzophenone	182	C13H10O	000119-61-9	87
5			Benzophenone	182	C13H10O	000119-61-9	76

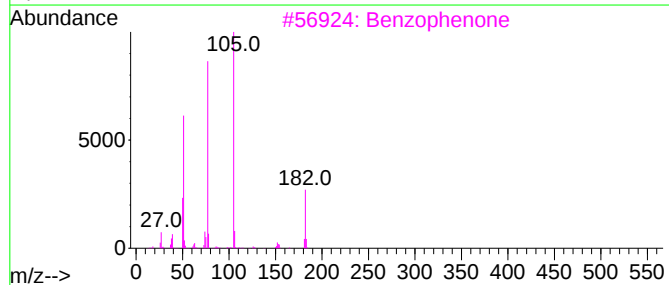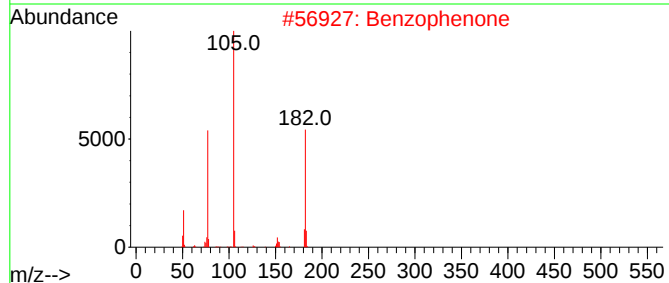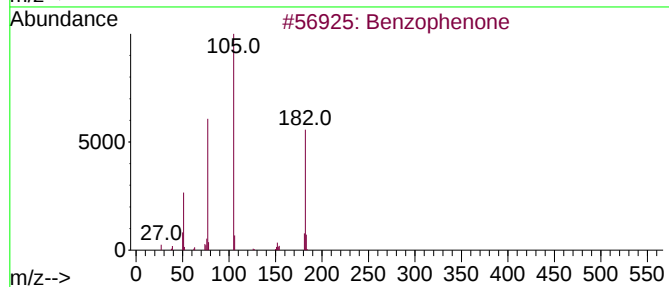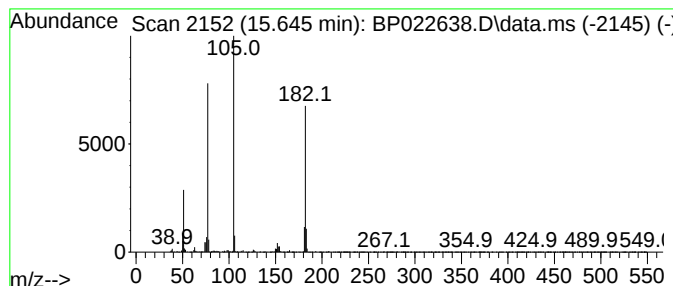

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022638.D
Acq On : 26 Oct 2024 11:58
Operator : RC/JU
Sample : P4532-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.645	2.2	ng/u1	135328	3	14.263	1227370	20.0