

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022642.D
 Acq On : 26 Oct 2024 14:40
 Operator : RC/JU
 Sample : PB164388BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK388

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	30	35	40	rBV	21413	30425	1.15%	0.114%
2	3.599	100	104	127	rBV	275279	453590	17.20%	1.697%
3	3.917	155	158	164	rVB	4734	7037	0.27%	0.026%
4	6.799	642	648	650	rBV2	3892	6158	0.23%	0.023%
5	6.846	650	656	668	rVV	361028	598640	22.69%	2.240%
6	6.993	675	681	692	rVB	275704	435198	16.50%	1.629%
7	7.193	708	715	724	rBV	371846	603569	22.88%	2.259%
8	7.646	786	792	804	rBV	349922	580688	22.01%	2.173%
9	8.358	904	913	927	rBV	437670	774587	29.36%	2.899%
10	8.793	978	987	997	rBV	348506	609563	23.11%	2.281%
11	9.199	1051	1056	1063	rBV4	7150	11521	0.44%	0.043%
12	9.505	1100	1108	1121	rBV	331656	549933	20.85%	2.058%
13	10.046	1192	1200	1216	rBV	481924	852972	32.34%	3.192%
14	10.199	1223	1226	1231	rVB6	1666	3137	0.12%	0.012%
15	10.410	1253	1262	1274	rVB	455400	807373	30.61%	3.021%
16	10.552	1278	1286	1301	rBV	418096	782336	29.66%	2.928%
17	11.675	1471	1477	1483	rVB5	5459	9376	0.36%	0.035%
18	11.999	1525	1532	1542	rBV5	5306	16021	0.61%	0.060%
19	13.675	1809	1817	1828	rBV	780864	1278972	48.49%	4.786%
20	13.957	1857	1865	1877	rBV	905470	1478935	56.07%	5.535%
21	14.269	1910	1918	1928	rBV	828132	1206674	45.75%	4.516%
22	14.510	1953	1959	1977	rBV	324948	575840	21.83%	2.155%
23	15.275	2083	2089	2101	rBV	1439258	1893173	71.77%	7.085%
24	15.428	2106	2115	2126	rBV	260982	519323	19.69%	1.943%
25	15.534	2129	2133	2138	rVB2	6781	10071	0.38%	0.038%
26	16.551	2302	2306	2311	rVB8	2421	4733	0.18%	0.018%
27	16.863	2355	2359	2363	rBV5	2716	4428	0.17%	0.017%
28	17.069	2383	2394	2403	rBV	936280	1558484	59.08%	5.832%
29	17.181	2403	2413	2425	rBV2	1336185	2121334	80.42%	7.939%
30	17.339	2437	2440	2445	rVB5	1891	3010	0.11%	0.011%
31	18.381	2613	2617	2620	rVB6	2472	3598	0.14%	0.013%
32	19.098	2735	2739	2745	rBV5	17053	27045	1.03%	0.101%
33	19.181	2749	2753	2762	rVV	19422	31748	1.20%	0.119%
34	19.557	2810	2817	2824	rBV	1839625	2570897	97.46%	9.621%
35	21.504	3142	3148	3161	rVB	1094908	1829848	69.37%	6.848%
36	24.545	3656	3665	3678	rVB	1030070	2637799	100.00%	9.872%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022642.D
Acq On : 26 Oct 2024 14:40
Operator : RC/JU
Sample : PB164388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK388

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.774	3694	3704	3718	rVB	708890	1833027	69.49%	6.860%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 26721063

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022642.D
Acq On : 26 Oct 2024 14:40
Operator : RC/JU
Sample : PB164388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

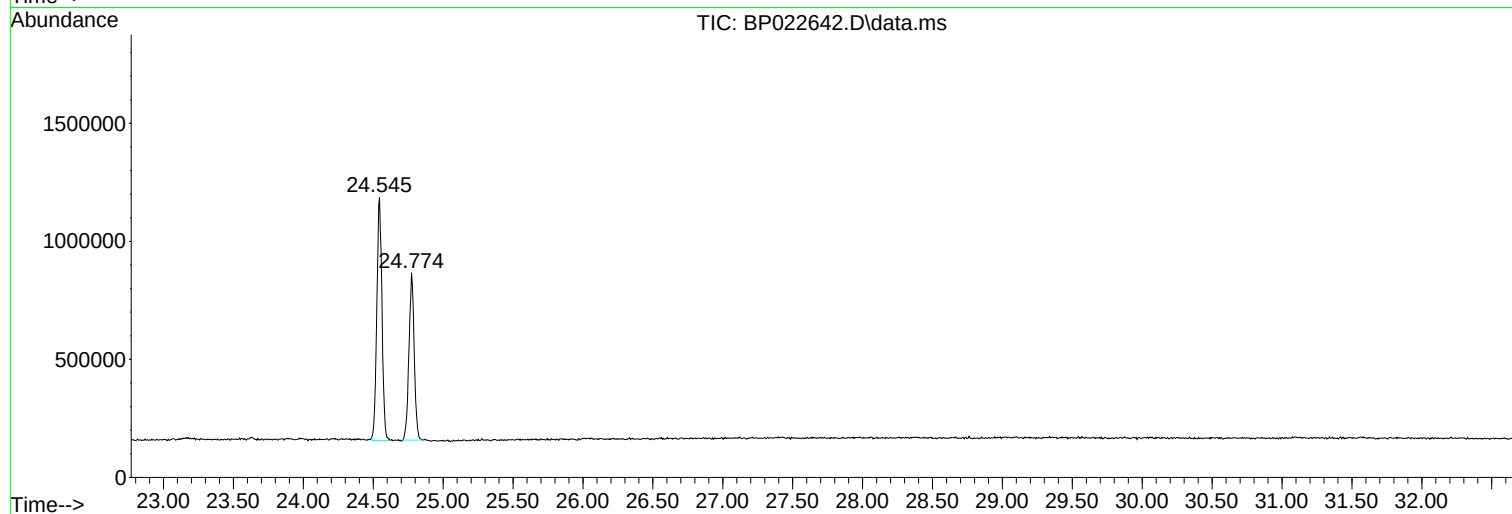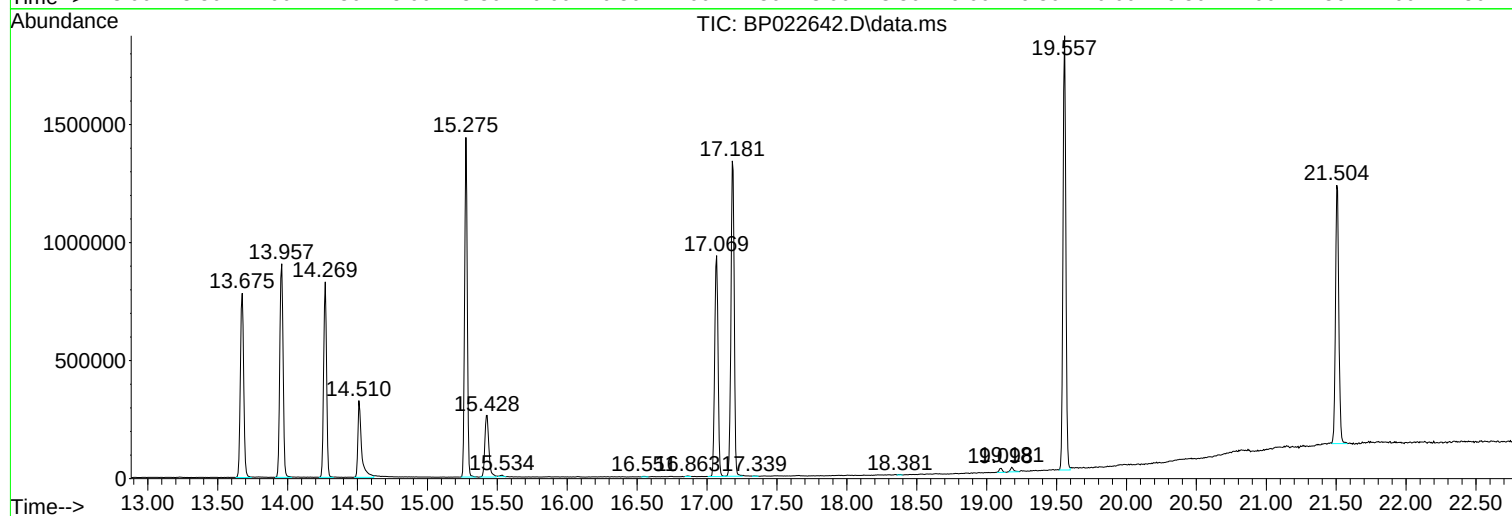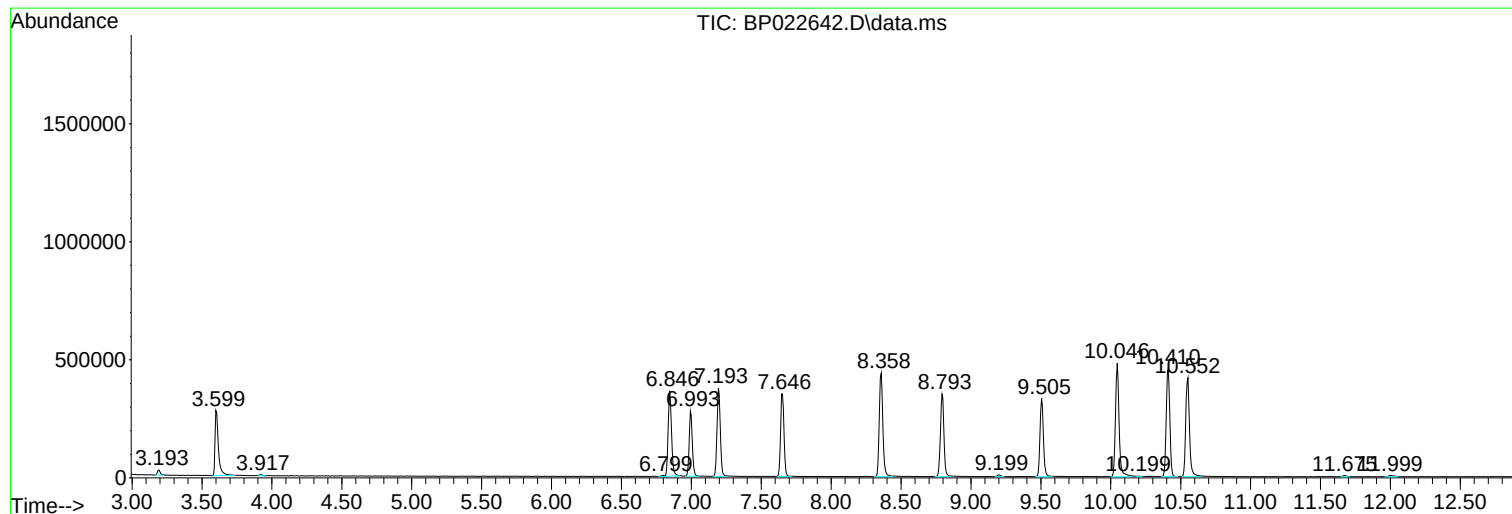

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022642.D
Acq On : 26 Oct 2024 14:40
Operator : RC/JU
Sample : PB164388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022642.D
Acq On : 26 Oct 2024 14:40
Operator : RC/JU
Sample : PB164388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc