

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022643.D
 Acq On : 26 Oct 2024 15:20
 Operator : RC/JU
 Sample : PB164387BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK387

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	40	rVB	18573	24206	0.95%	0.106%
2	3.599	100	104	127	rBV	249225	390675	15.27%	1.710%
3	3.911	153	157	165	rBV4	4518	7792	0.30%	0.034%
4	6.799	643	648	650	rBV4	3027	4194	0.16%	0.018%
5	6.840	650	655	671	rVV	301063	514822	20.13%	2.254%
6	6.993	674	681	691	rVB	240014	357170	13.96%	1.564%
7	7.193	706	715	728	rBV	309489	510491	19.96%	2.235%
8	7.646	785	792	803	rVB	282249	457029	17.87%	2.001%
9	8.352	905	912	930	rBV	371308	648157	25.34%	2.837%
10	8.793	978	987	997	rBV	302811	516382	20.19%	2.261%
11	9.193	1051	1055	1063	rVB6	3493	6433	0.25%	0.028%
12	9.504	1100	1108	1119	rBV2	261703	465425	18.20%	2.037%
13	10.046	1191	1200	1216	rBV	384315	712266	27.85%	3.118%
14	10.404	1253	1261	1271	rBV	359342	620896	24.27%	2.718%
15	10.546	1278	1285	1303	rBV	366962	648395	25.35%	2.838%
16	11.669	1472	1476	1483	rBV3	2820	4244	0.17%	0.019%
17	12.004	1527	1533	1538	rBV3	5199	10505	0.41%	0.046%
18	13.228	1736	1741	1745	rBV6	1505	2960	0.12%	0.013%
19	13.663	1806	1815	1829	rBV	684351	1043045	40.78%	4.566%
20	13.945	1856	1863	1878	rBV	738711	1201178	46.96%	5.258%
21	14.263	1910	1917	1930	rBV	665835	927085	36.25%	4.058%
22	14.516	1952	1960	1984	rBV	248481	529561	20.70%	2.318%
23	15.275	2083	2089	2103	rBV	1147928	1558404	60.93%	6.822%
24	15.416	2105	2113	2128	rBV	243092	447246	17.49%	1.958%
25	15.528	2128	2132	2138	rVB7	5111	10094	0.39%	0.044%
26	16.075	2222	2225	2230	rVB7	1901	2575	0.10%	0.011%
27	16.551	2302	2306	2311	rVB8	1678	3038	0.12%	0.013%
28	16.857	2352	2358	2359	rBV5	2470	3992	0.16%	0.017%
29	17.063	2385	2393	2404	rBV	960944	1249231	48.84%	5.469%
30	17.175	2404	2412	2425	rVV	1063896	1800001	70.37%	7.880%
31	19.098	2736	2739	2746	rVB3	16832	23598	0.92%	0.103%
32	19.175	2748	2752	2756	rVV2	14120	21289	0.83%	0.093%
33	19.551	2810	2816	2825	rBV	1768635	2345197	91.69%	10.266%
34	21.510	3142	3149	3158	rBV	895017	1558932	60.95%	6.824%
35	24.551	3657	3666	3680	rVB	987481	2557786	100.00%	11.197%
36	24.774	3695	3704	3717	rVB2	571372	1659274	64.87%	7.264%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022643.D
Acq On : 26 Oct 2024 15:20
Operator : RC/JU
Sample : PB164387BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK387

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 22843568

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022643.D
Acq On : 26 Oct 2024 15:20
Operator : RC/JU
Sample : PB164387BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK387

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

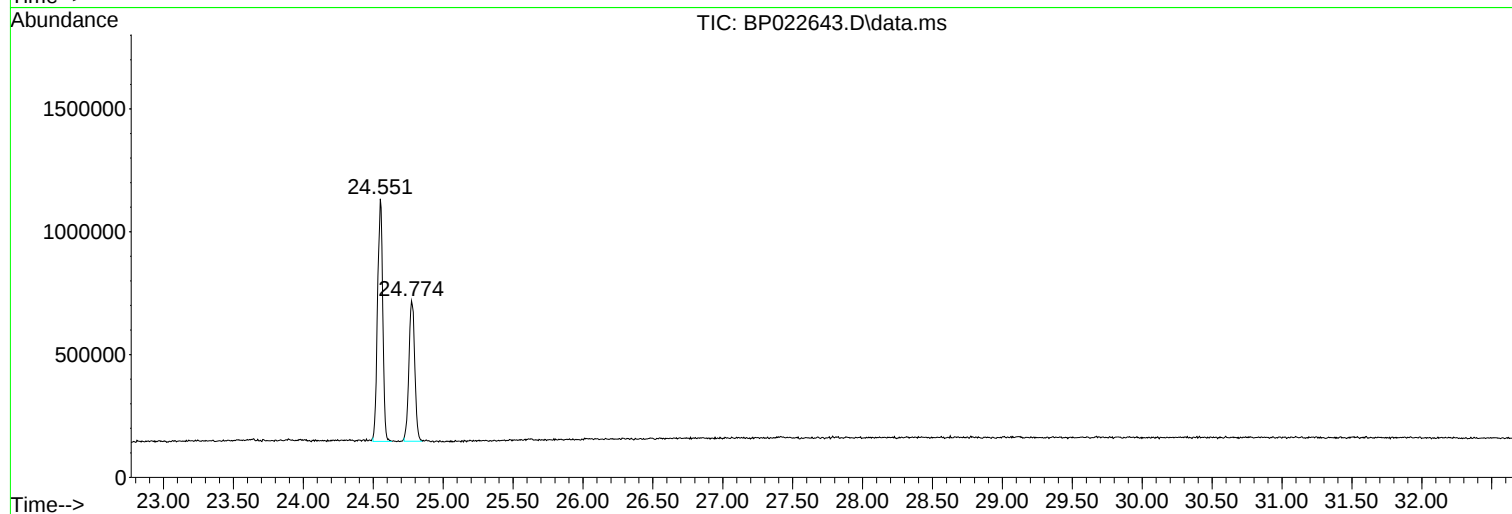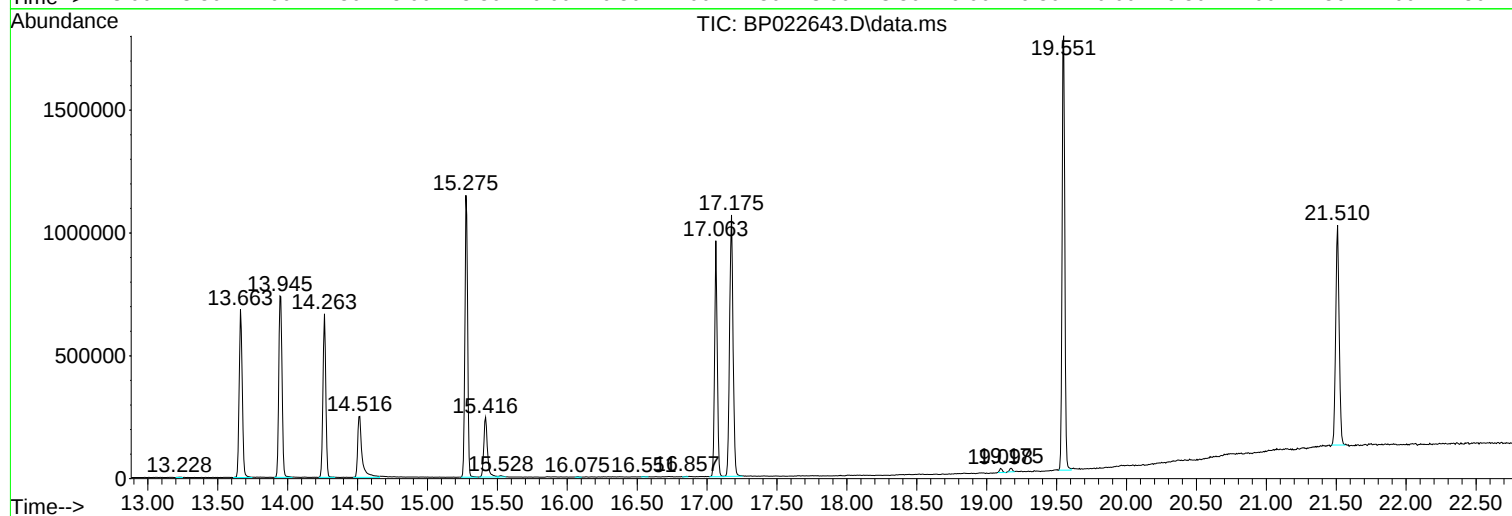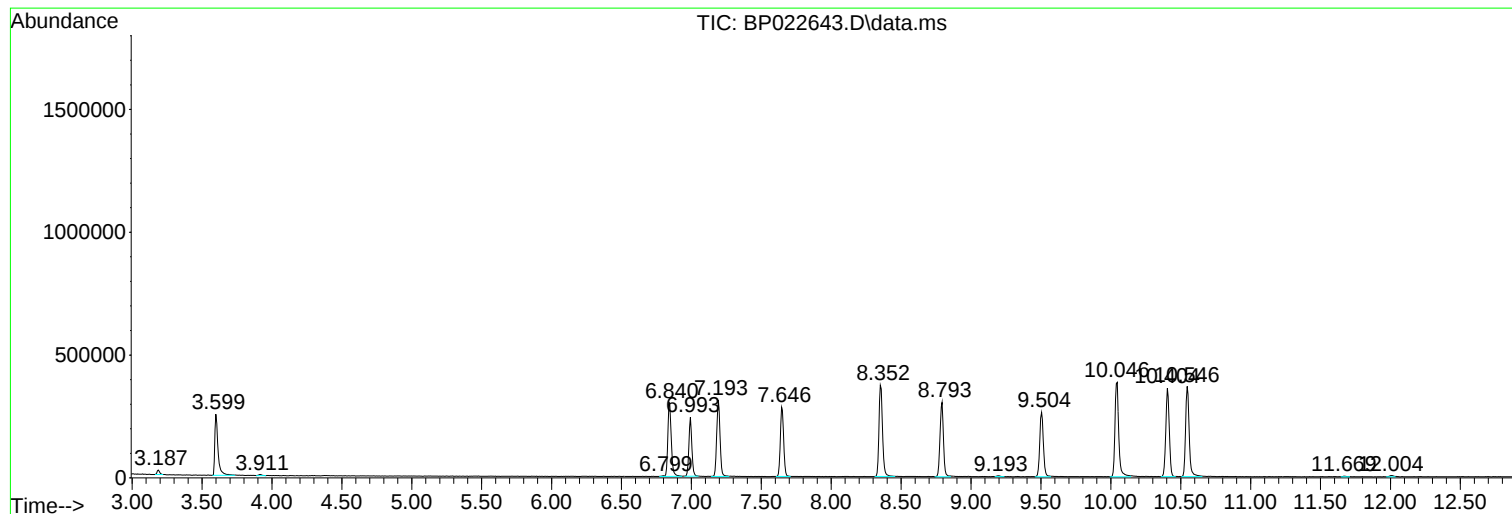

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022643.D
Acq On : 26 Oct 2024 15:20
Operator : RC/JU
Sample : PB164387BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK387

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022643.D
Acq On : 26 Oct 2024 15:20
Operator : RC/JU
Sample : PB164387BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK387

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc