

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022649.D
 Acq On : 26 Oct 2024 19:23
 Operator : RC/JU
 Sample : P4532-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	38	rBV	16208	19687	0.59%	0.075%
2	3.611	102	106	122	rBV	58948	114399	3.42%	0.433%
3	3.917	153	158	165	rVB3	5312	7694	0.23%	0.029%
4	4.281	217	220	228	rVB8	4580	8721	0.26%	0.033%
5	4.358	228	233	237	rBV7	2024	3988	0.12%	0.015%
6	4.464	245	251	252	rBV5	2101	3373	0.10%	0.013%
7	5.499	422	427	431	rBV6	5941	9919	0.30%	0.038%
8	5.711	455	463	465	rBV9	2326	4980	0.15%	0.019%
9	5.817	475	481	487	rVB8	3240	4970	0.15%	0.019%
10	6.028	511	517	523	rBV2	19933	34967	1.04%	0.132%
11	6.246	550	554	555	rBV3	3448	4409	0.13%	0.017%
12	6.264	555	557	565	rVB5	4536	6718	0.20%	0.025%
13	6.422	579	584	588	rBV7	1674	3374	0.10%	0.013%
14	6.475	588	593	597	rVV2	8087	13608	0.41%	0.052%
15	6.522	597	601	608	rVB	12643	19066	0.57%	0.072%
16	6.846	650	656	667	rBV	87111	157522	4.70%	0.596%
17	6.993	675	681	692	rBV	236658	370258	11.06%	1.402%
18	7.193	707	715	728	rBV	303518	499390	14.92%	1.891%
19	7.652	786	793	803	rBV	325514	534501	15.96%	2.024%
20	8.358	905	913	929	rBV	266760	458263	13.69%	1.735%
21	8.793	979	987	995	rBV	330362	551236	16.46%	2.087%
22	9.193	1050	1055	1060	rBV7	2826	4702	0.14%	0.018%
23	9.358	1078	1083	1088	rBV9	2482	4373	0.13%	0.017%
24	9.505	1100	1108	1122	rBV	275144	489239	14.61%	1.852%
25	9.781	1151	1155	1160	rVB7	2398	4725	0.14%	0.018%
26	10.040	1192	1199	1215	rBV	441647	762044	22.76%	2.885%
27	10.405	1253	1261	1270	rBV	431257	726761	21.71%	2.752%
28	10.546	1273	1285	1300	rBV	297864	596164	17.81%	2.257%
29	11.222	1395	1400	1404	rBV6	4814	10598	0.32%	0.040%
30	11.669	1472	1476	1483	rVB8	2348	3864	0.12%	0.015%
31	12.004	1526	1533	1539	rBV4	6499	11592	0.35%	0.044%
32	12.863	1675	1679	1683	rBV4	2405	3460	0.10%	0.013%
33	13.675	1811	1817	1833	rVB	952147	1252748	37.42%	4.743%
34	13.957	1858	1865	1878	rBV	953140	1339236	40.00%	5.071%
35	14.269	1911	1918	1926	rBV	731145	1093398	32.66%	4.140%
36	14.528	1955	1962	1977	rBV2	57529	179432	5.36%	0.679%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022649.D
 Acq On : 26 Oct 2024 19:23
 Operator : RC/JU
 Sample : P4532-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNX0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.081	2051	2056	2057	rBV2	3760	4942	0.15%	0.019%
38	15.098	2057	2059	2063	rVB3	3942	4838	0.14%	0.018%
39	15.287	2083	2091	2097	rBV	1366966	1884956	56.30%	7.137%
40	15.340	2097	2100	2105	rVV5	9513	16115	0.48%	0.061%
41	15.416	2107	2113	2126	rVV	469610	652834	19.50%	2.472%
42	15.528	2128	2132	2139	rVB6	5677	11991	0.36%	0.045%
43	15.663	2148	2155	2163	rVB	74253	107189	3.20%	0.406%
44	15.863	2186	2189	2197	rVB9	2377	3836	0.11%	0.015%
45	16.010	2210	2214	2221	rVV	10788	14920	0.45%	0.056%
46	16.075	2223	2225	2231	rVB6	3159	4853	0.14%	0.018%
47	16.234	2246	2252	2257	rBV	21235	35879	1.07%	0.136%
48	16.281	2257	2260	2263	rVB2	3533	3747	0.11%	0.014%
49	16.734	2335	2337	2342	rBV6	2970	3713	0.11%	0.014%
50	16.851	2350	2357	2361	rBV5	4002	8652	0.26%	0.033%
51	17.004	2377	2383	2386	rBV7	3321	5719	0.17%	0.022%
52	17.075	2389	2395	2401	rVV	1142838	1451600	43.35%	5.496%
53	17.163	2404	2410	2425	rVB	1595679	2369991	70.78%	8.973%
54	17.369	2442	2445	2447	rBV2	3420	3668	0.11%	0.014%
55	17.757	2508	2511	2517	rBV8	5041	7410	0.22%	0.028%
56	17.881	2527	2532	2534	rBV6	3387	5517	0.16%	0.021%
57	18.010	2549	2554	2559	rBV3	43643	60356	1.80%	0.229%
58	18.081	2562	2566	2570	rVB	11618	16205	0.48%	0.061%
59	18.469	2625	2632	2635	rBV7	5823	13337	0.40%	0.050%
60	18.875	2697	2701	2707	rVB2	12202	19797	0.59%	0.075%
61	19.098	2736	2739	2745	rVB5	19095	27789	0.83%	0.105%
62	19.175	2748	2752	2755	rBV	28501	40381	1.21%	0.153%
63	19.216	2755	2759	2771	rVB4	46906	86408	2.58%	0.327%
64	19.333	2776	2779	2785	rVV3	25201	31510	0.94%	0.119%
65	19.551	2810	2816	2826	rBV	2459239	3040997	90.83%	11.514%
66	21.498	3141	3147	3161	rVB	1306995	1872403	55.92%	7.089%
67	24.533	3654	3663	3674	rVB	1454024	3348184	100.00%	12.677%
68	24.757	3692	3701	3712	rVB	695820	1938971	57.91%	7.341%




Sum of corrected areas: 26412087

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022649.D
Acq On : 26 Oct 2024 19:23
Operator : RC/JU
Sample : P4532-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

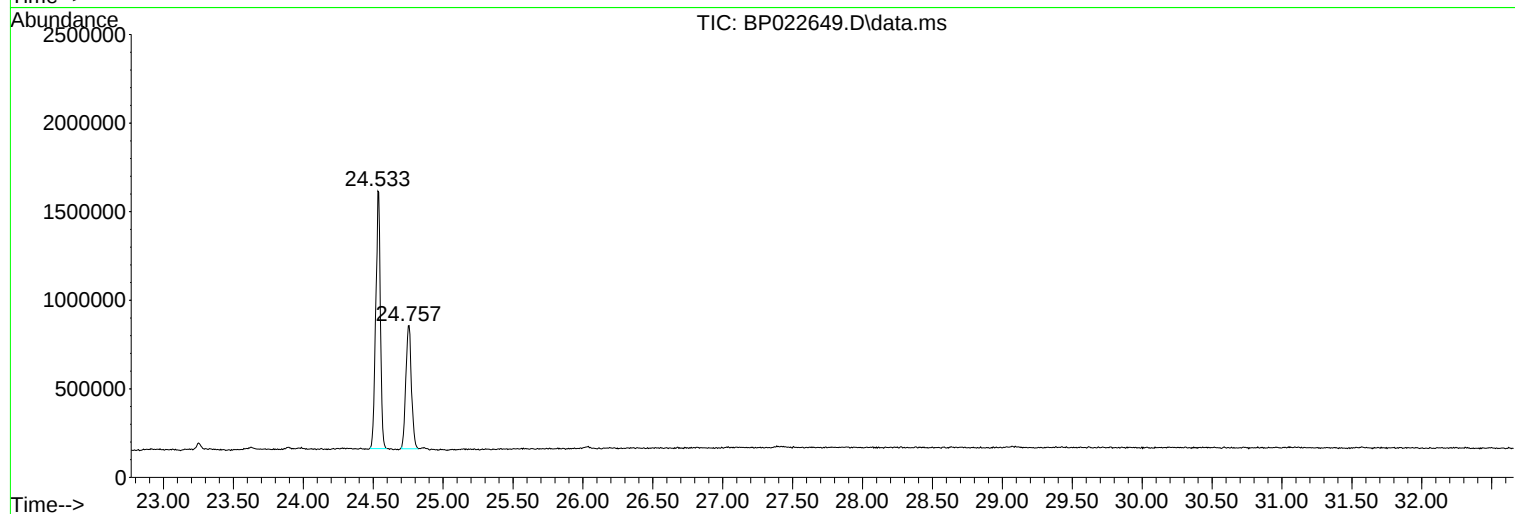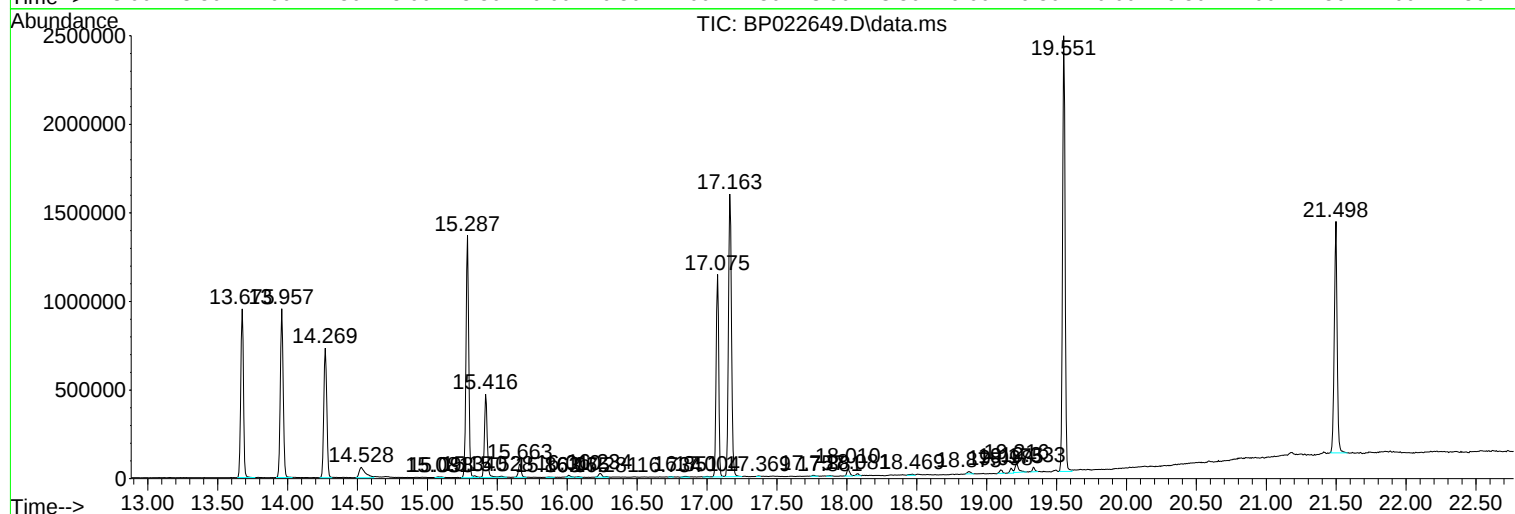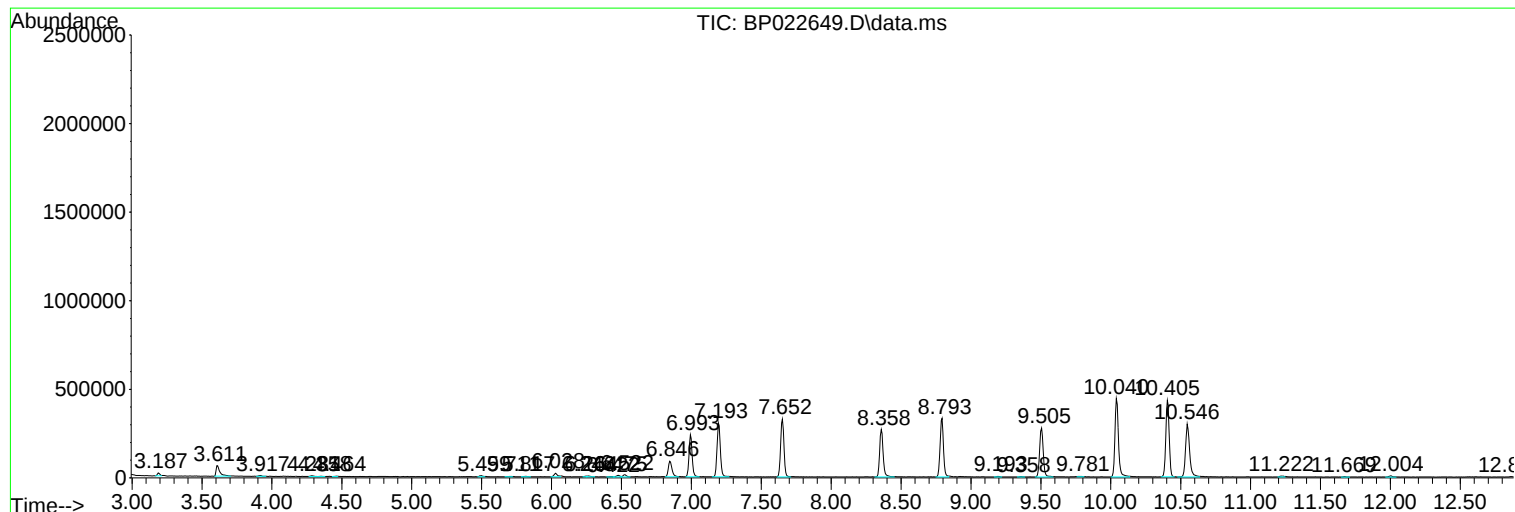

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022649.D
Acq On : 26 Oct 2024 19:23
Operator : RC/JU
Sample : P4532-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022649.D
Acq On : 26 Oct 2024 19:23
Operator : RC/JU
Sample : P4532-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc