

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022651.D
 Acq On : 26 Oct 2024 20:44
 Operator : RC/JU
 Sample : P4532-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	40	rBV	17211	21543	0.62%	0.080%
2	3.605	101	105	113	rBV	75716	119867	3.45%	0.444%
3	3.916	154	158	165	rVB2	4882	8515	0.25%	0.032%
4	4.275	216	219	224	rBV6	3287	4766	0.14%	0.018%
5	4.993	336	341	347	rVB7	2501	4409	0.13%	0.016%
6	5.493	421	426	430	rBV3	7531	11493	0.33%	0.043%
7	5.710	458	463	466	rVB7	2767	3772	0.11%	0.014%
8	5.816	475	481	486	rBV8	2655	4064	0.12%	0.015%
9	6.022	510	516	521	rBV2	20770	36409	1.05%	0.135%
10	6.246	549	554	555	rBV4	3905	5176	0.15%	0.019%
11	6.475	587	593	596	rBV5	8359	13757	0.40%	0.051%
12	6.516	596	600	607	rVB2	13968	21109	0.61%	0.078%
13	6.793	644	647	650	rBV3	4462	5357	0.15%	0.020%
14	6.846	650	656	669	rVB	92532	162664	4.69%	0.603%
15	6.987	673	680	692	rBV	261097	431152	12.42%	1.599%
16	7.187	708	714	724	rBV	316057	527012	15.18%	1.954%
17	7.645	785	792	805	rBV	319813	521569	15.02%	1.934%
18	8.351	905	912	926	rBV	280735	465259	13.40%	1.725%
19	8.787	978	986	995	rBV	356189	600966	17.31%	2.228%
20	9.187	1050	1054	1062	rVB4	13612	21994	0.63%	0.082%
21	9.504	1099	1108	1122	rBV	312778	556649	16.03%	2.064%
22	9.775	1149	1154	1160	rVB9	1880	4405	0.13%	0.016%
23	10.039	1189	1199	1216	rBV	468024	843250	24.29%	3.127%
24	10.398	1252	1260	1274	rVB	417775	711939	20.51%	2.640%
25	10.545	1278	1285	1302	rBV	309131	614232	17.69%	2.277%
26	10.763	1318	1322	1328	rVB6	2999	5213	0.15%	0.019%
27	11.222	1391	1400	1410	rBV6	4190	14014	0.40%	0.052%
28	11.675	1470	1477	1483	rBV4	7754	13045	0.38%	0.048%
29	11.998	1526	1532	1540	rBV3	7280	14046	0.40%	0.052%
30	13.151	1725	1728	1733	rVB7	3686	4872	0.14%	0.018%
31	13.663	1808	1815	1827	rBV	874280	1320772	38.04%	4.897%
32	13.945	1852	1863	1875	rBV	1037859	1438576	41.43%	5.334%
33	14.257	1909	1916	1924	rBV	778543	1054672	30.38%	3.911%
34	14.516	1953	1960	1974	rBV2	72708	159817	4.60%	0.593%
35	15.274	2082	2089	2095	rBV	1380685	1959143	56.43%	7.264%
36	15.322	2095	2097	2104	rVB6	7761	11587	0.33%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022651.D
 Acq On : 26 Oct 2024 20:44
 Operator : RC/JU
 Sample : P4532-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNX2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.416	2106	2113	2126	rBV	460824	686070	19.76%	2.544%
38	15.527	2128	2132	2138	rVB6	6759	12212	0.35%	0.045%
39	15.639	2146	2151	2159	rVB	39423	61721	1.78%	0.229%
40	15.857	2182	2188	2191	rBV8	3124	6200	0.18%	0.023%
41	15.986	2206	2210	2216	rBV2	10191	15788	0.45%	0.059%
42	16.222	2245	2250	2258	rVB2	17746	26750	0.77%	0.099%
43	16.469	2288	2292	2297	rBV6	5792	9323	0.27%	0.035%
44	16.533	2298	2303	2308	rVV8	6178	9952	0.29%	0.037%
45	16.645	2316	2322	2326	rBV3	22391	35989	1.04%	0.133%
46	16.833	2349	2354	2359	rBV8	3613	8170	0.24%	0.030%
47	16.980	2375	2379	2383	rBV6	2437	3544	0.10%	0.013%
48	17.057	2385	2392	2398	rBV	1082860	1422515	40.97%	5.274%
49	17.157	2402	2409	2422	rVV2	1575768	2385802	68.72%	8.846%
50	17.245	2422	2424	2429	rVB5	4141	5408	0.16%	0.020%
51	17.357	2440	2443	2448	rVB2	6312	8190	0.24%	0.030%
52	17.463	2456	2461	2463	rBV6	2776	4824	0.14%	0.018%
53	17.751	2506	2510	2514	rBV7	3864	7184	0.21%	0.027%
54	17.863	2527	2529	2533	rBV5	4058	5263	0.15%	0.020%
55	17.986	2545	2550	2556	rBV2	40854	61718	1.78%	0.229%
56	18.057	2559	2562	2567	rVB	30204	37832	1.09%	0.140%
57	18.292	2595	2602	2608	rBV9	7100	22183	0.64%	0.082%
58	18.433	2624	2626	2632	rVB7	5754	7996	0.23%	0.030%
59	19.092	2734	2738	2742	rBV3	22086	29543	0.85%	0.110%
60	19.163	2746	2750	2753	rVV2	26848	34710	1.00%	0.129%
61	19.204	2753	2757	2767	rVB7	23328	50988	1.47%	0.189%
62	19.321	2774	2777	2787	rVB5	24152	30626	0.88%	0.114%
63	19.539	2808	2814	2822	rBV	2188267	3098020	89.23%	11.487%
64	21.486	3139	3145	3160	rVB	1048784	1829643	52.70%	6.784%
65	24.521	3652	3661	3671	rVB	1457900	3472006	100.00%	12.874%
66	24.739	3689	3698	3711	rVB	634926	1862783	53.65%	6.907%




Sum of corrected areas: 26970038

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022651.D
Acq On : 26 Oct 2024 20:44
Operator : RC/JU
Sample : P4532-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

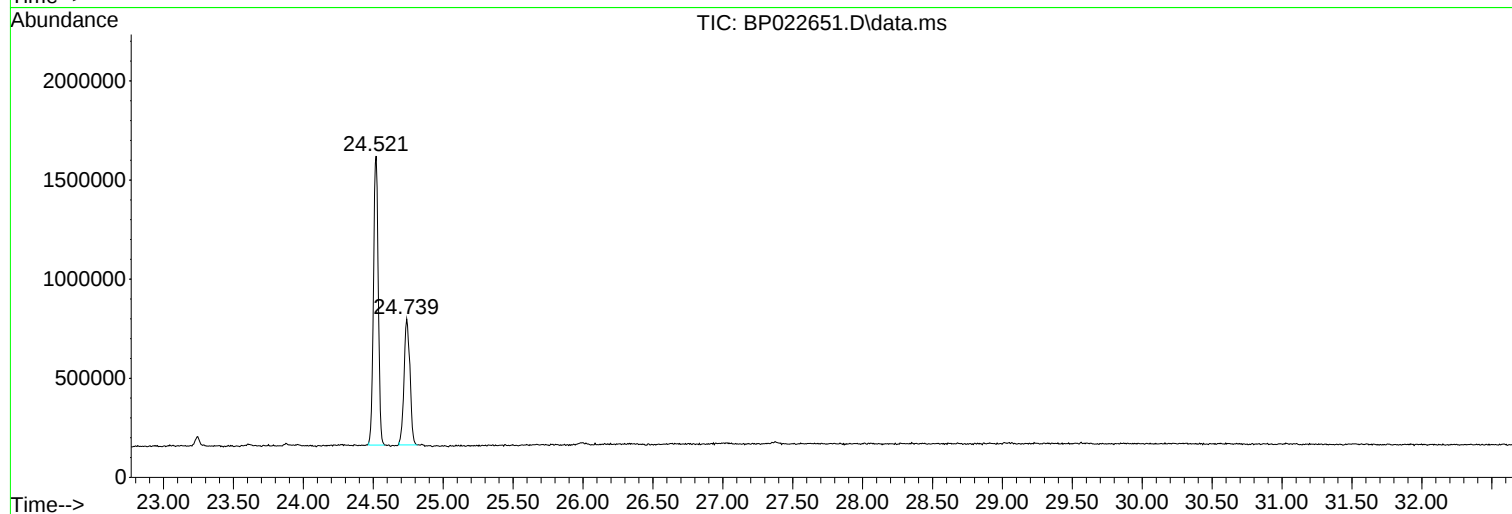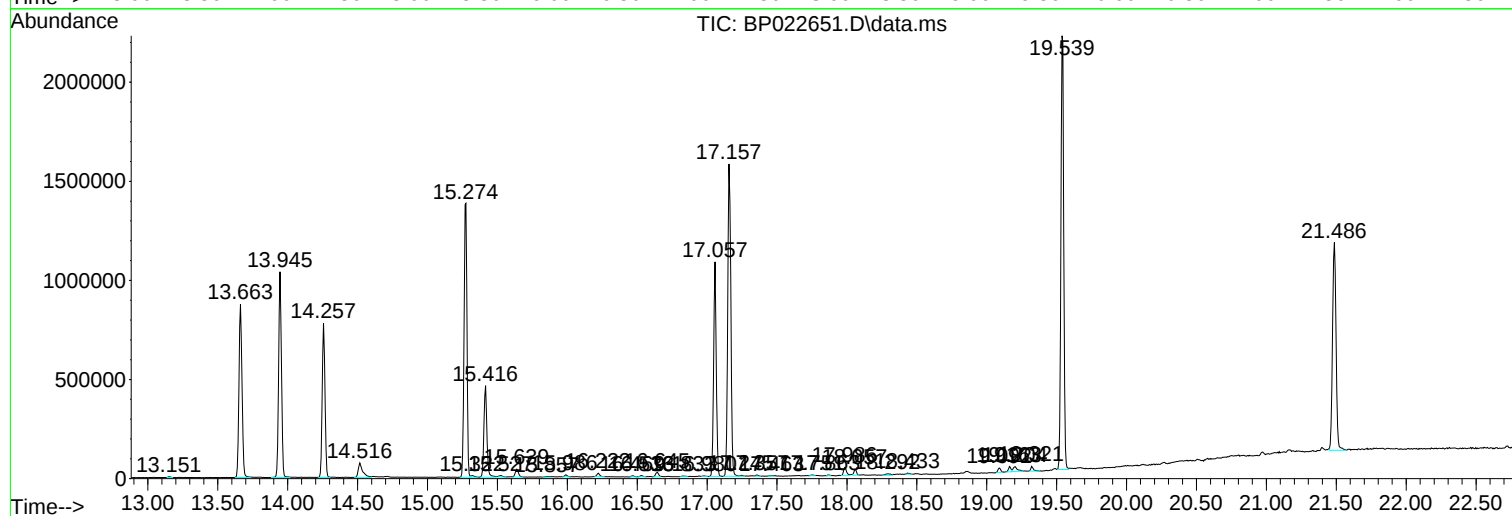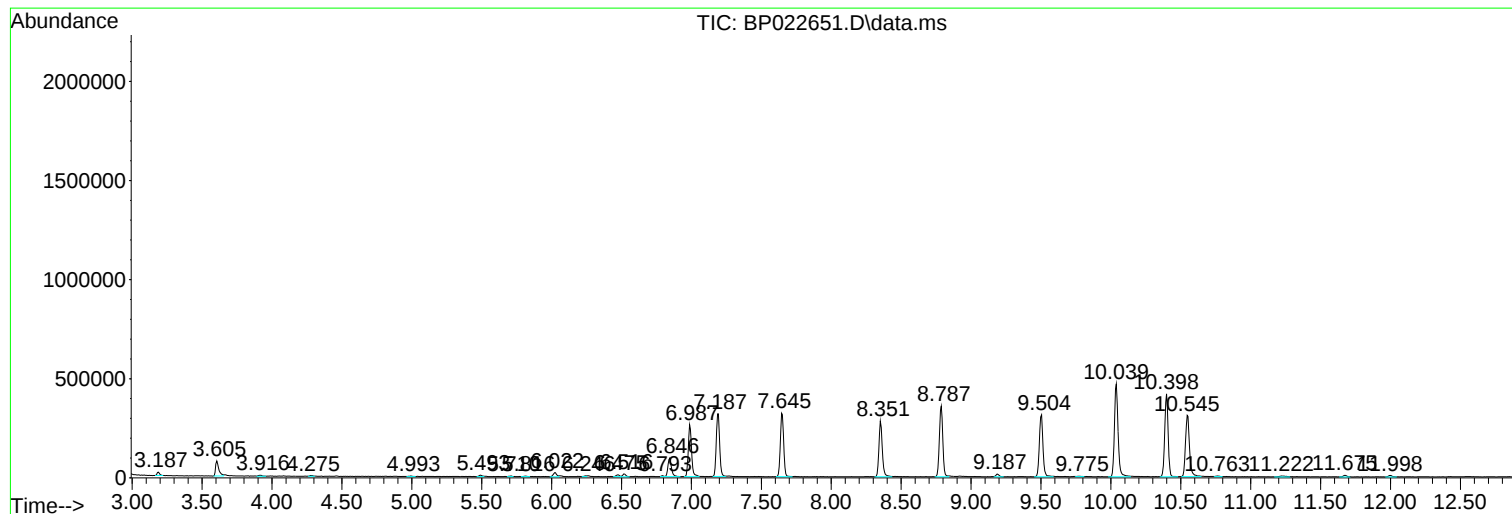

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022651.D
Acq On : 26 Oct 2024 20:44
Operator : RC/JU
Sample : P4532-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022651.D
Acq On : 26 Oct 2024 20:44
Operator : RC/JU
Sample : P4532-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc