

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022659.D
 Acq On : 27 Oct 2024 02:49
 Operator : RC/JU
 Sample : PB164421BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK421

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022659.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	41	rVB	18302	25333	1.07%	0.120%
2	3.599	100	104	117	rBV	212666	357117	15.04%	1.696%
3	3.910	153	157	164	rBV3	4008	6660	0.28%	0.032%
4	6.793	643	647	649	rBV5	2069	3705	0.16%	0.018%
5	6.840	649	655	674	rVB	278861	477224	20.10%	2.266%
6	6.987	674	680	689	rBV	202133	324014	13.65%	1.538%
7	7.187	707	714	731	rBV	273413	475224	20.02%	2.256%
8	7.645	782	792	803	rBV	259784	414000	17.44%	1.966%
9	8.351	902	912	926	rBV	354386	597665	25.17%	2.838%
10	8.787	977	986	996	rBV	278792	478345	20.15%	2.271%
11	9.192	1051	1055	1062	rVB4	3704	5986	0.25%	0.028%
12	9.498	1099	1107	1117	rBV	241743	424996	17.90%	2.018%
13	10.039	1191	1199	1212	rBV	363850	641747	27.03%	3.047%
14	10.398	1252	1260	1270	rBV	313294	560002	23.59%	2.659%
15	10.539	1275	1284	1305	rBV	319522	598404	25.20%	2.841%
16	11.669	1470	1476	1482	rVB9	3273	5571	0.23%	0.026%
17	11.998	1526	1532	1537	rBV5	4675	9015	0.38%	0.043%
18	13.669	1809	1816	1826	rBV	720749	984178	41.45%	4.673%
19	13.951	1856	1864	1877	rBV	760015	1103245	46.47%	5.238%
20	14.263	1909	1917	1927	rBV	542387	835619	35.19%	3.967%
21	14.498	1951	1957	1984	rBV	233094	496992	20.93%	2.360%
22	15.269	2081	2088	2102	rBV	891528	1440610	60.68%	6.840%
23	15.410	2106	2112	2124	rVV	307409	423634	17.84%	2.011%
24	15.516	2126	2130	2135	rVB8	4837	8471	0.36%	0.040%
25	16.833	2353	2354	2362	rVB8	2462	3602	0.15%	0.017%
26	17.068	2385	2394	2403	rBV	718026	1131252	47.65%	5.371%
27	17.163	2404	2410	2425	rVB	1327548	1726100	72.70%	8.195%
28	19.092	2734	2738	2744	rBV4	13172	22125	0.93%	0.105%
29	19.168	2748	2751	2755	rVV2	14344	18760	0.79%	0.089%
30	19.545	2809	2815	2824	rBV	1706481	2186887	92.11%	10.383%
31	21.498	3141	3147	3157	rVB	894662	1408840	59.34%	6.689%
32	24.527	3653	3662	3676	rVB	867802	2374263	100.00%	11.273%
33	24.750	3691	3700	3713	rVB	605995	1492647	62.87%	7.087%




Sum of corrected areas: 21062233

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022659.D
Acq On : 27 Oct 2024 02:49
Operator : RC/JU
Sample : PB164421BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

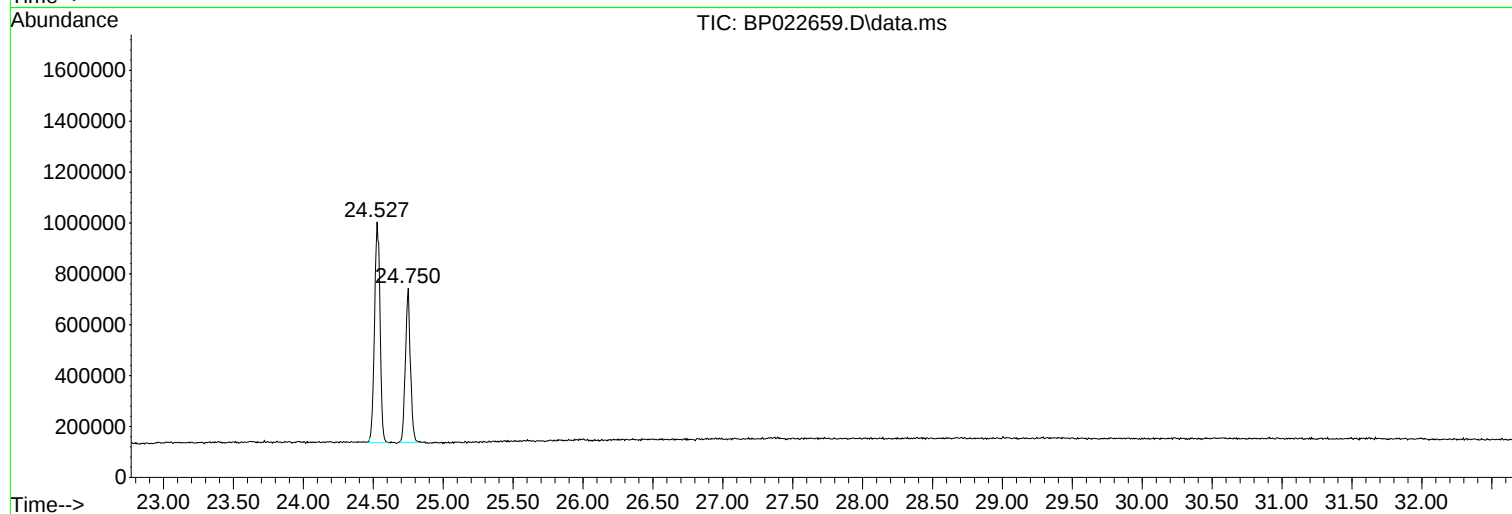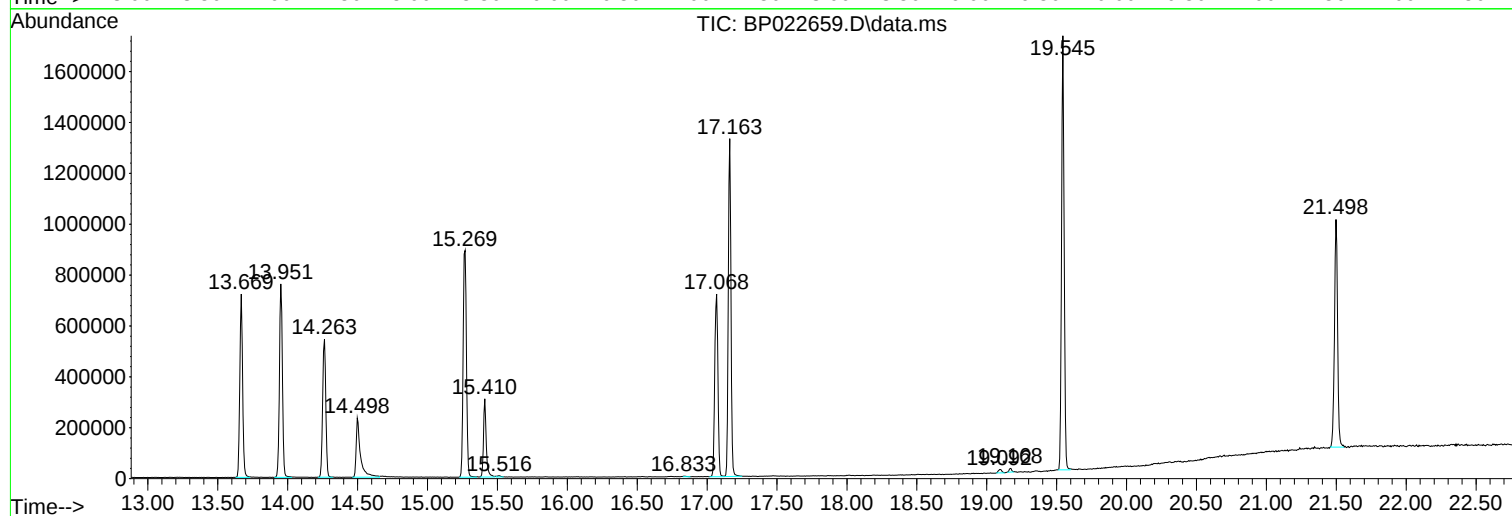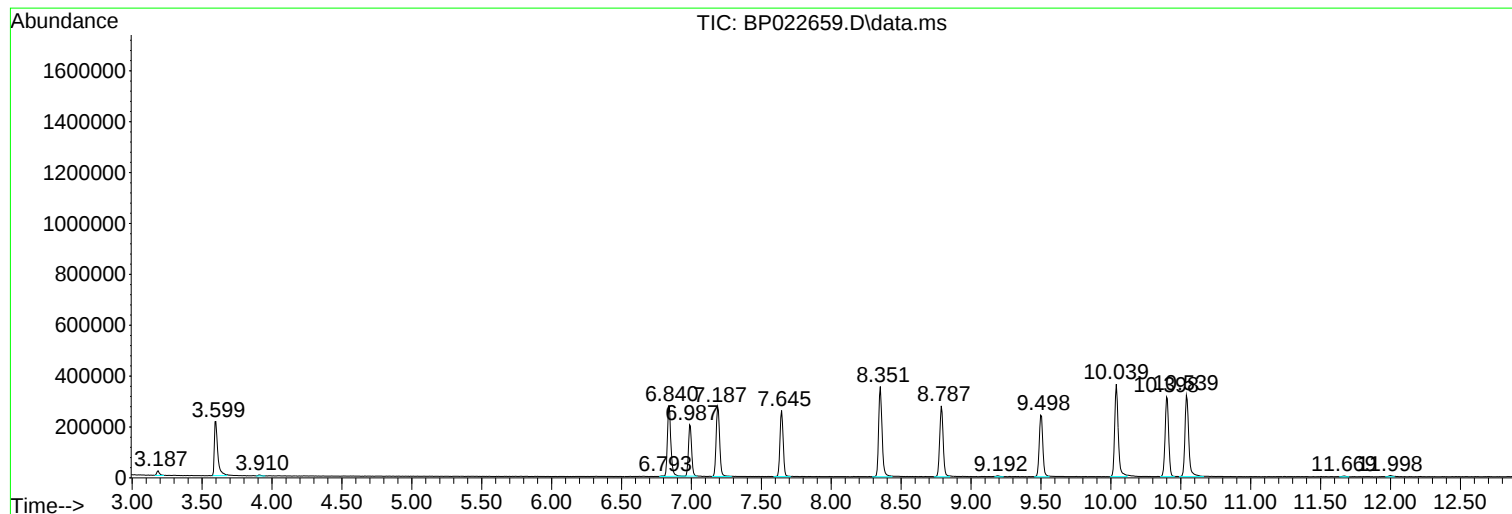

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022659.D
Acq On : 27 Oct 2024 02:49
Operator : RC/JU
Sample : PB164421BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022659.D
Acq On : 27 Oct 2024 02:49
Operator : RC/JU
Sample : PB164421BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc