

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022660.D
 Acq On : 27 Oct 2024 03:30
 Operator : RC/JU
 Sample : P4559-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNY0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022660.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	30	33	43	rVB	15223	21473	0.73%	0.097%
2	3.611	102	106	118	rBV	26211	49122	1.67%	0.221%
3	3.911	152	157	159	rBV3	3677	4890	0.17%	0.022%
4	4.822	307	312	320	rVB5	2623	6237	0.21%	0.028%
5	6.793	641	647	651	rBV2	5456	9453	0.32%	0.043%
6	6.846	651	656	667	rVB2	63473	116447	3.97%	0.524%
7	6.987	672	680	692	rVV	216283	336094	11.45%	1.512%
8	7.193	704	715	727	rBV	244399	423123	14.42%	1.904%
9	7.646	785	792	799	rBV	218891	366749	12.50%	1.650%
10	7.710	799	803	820	rVB2	31855	64771	2.21%	0.291%
11	8.352	905	912	926	rBV	204588	369307	12.59%	1.662%
12	8.787	979	986	996	rBV	304022	498334	16.98%	2.243%
13	9.193	1048	1055	1062	rBV2	35707	55129	1.88%	0.248%
14	9.499	1099	1107	1119	rBV	259601	444693	15.15%	2.001%
15	10.040	1190	1199	1214	rBV	388418	675576	23.02%	3.040%
16	10.399	1253	1260	1271	rVB	296743	499878	17.03%	2.250%
17	10.546	1277	1285	1301	rBV	221693	393919	13.42%	1.773%
18	11.663	1469	1475	1482	rBV2	19251	30005	1.02%	0.135%
19	11.998	1525	1532	1541	rBV3	4967	10524	0.36%	0.047%
20	12.610	1630	1636	1640	rBV8	2445	4161	0.14%	0.019%
21	12.857	1674	1678	1683	rBV6	2641	4722	0.16%	0.021%
22	13.669	1810	1816	1826	rBV	833320	1074380	36.61%	4.835%
23	13.951	1855	1864	1876	rBV2	723864	1157498	39.45%	5.209%
24	14.257	1910	1916	1927	rBV	521483	770260	26.25%	3.466%
25	14.528	1955	1962	1973	rBV2	38535	108812	3.71%	0.490%
26	15.069	2049	2054	2061	rBV	112872	154175	5.25%	0.694%
27	15.275	2082	2089	2096	rBV	1172590	1593906	54.32%	7.173%
28	15.328	2096	2098	2105	rVV4	13340	21411	0.73%	0.096%
29	15.410	2106	2112	2124	rVV	390528	534334	18.21%	2.405%
30	15.516	2127	2130	2137	rVB8	5709	11621	0.40%	0.052%
31	15.651	2149	2153	2159	rBV3	8787	11565	0.39%	0.052%
32	15.792	2171	2177	2182	rBV10	2599	6017	0.21%	0.027%
33	16.010	2209	2214	2219	rBV	3709	6730	0.23%	0.030%
34	16.128	2229	2234	2240	rVB5	3129	6612	0.23%	0.030%
35	16.228	2246	2251	2256	rBV9	1593	3120	0.11%	0.014%
36	16.663	2321	2325	2328	rVB6	3762	4622	0.16%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022660.D
 Acq On : 27 Oct 2024 03:30
 Operator : RC/JU
 Sample : P4559-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	16.733	2334	2337	2344	rVB8	3172	4559	0.16%	0.021%
38	16.839	2350	2355	2356	rBV5	2431	3305	0.11%	0.015%
39	17.063	2388	2393	2402	rVB	807337	1043249	35.55%	4.695%
40	17.163	2403	2410	2425	rVV2	1225413	1932236	65.85%	8.695%
41	17.275	2427	2429	2434	rVB5	2323	3266	0.11%	0.015%
42	17.363	2438	2444	2450	rVV2	6955	11733	0.40%	0.053%
43	17.451	2453	2459	2468	rBV10	5629	15122	0.52%	0.068%
44	18.004	2549	2553	2558	rBV3	19343	27300	0.93%	0.123%
45	18.069	2561	2564	2570	rVB	9243	11611	0.40%	0.052%
46	19.010	2722	2724	2727	rBV3	3041	4201	0.14%	0.019%
47	19.104	2736	2740	2744	rBV4	18670	26081	0.89%	0.117%
48	19.175	2748	2752	2755	rBV	18286	26163	0.89%	0.118%
49	19.216	2755	2759	2763	rBV2	30804	41862	1.43%	0.188%
50	19.339	2777	2780	2790	rBV8	16271	25763	0.88%	0.116%
51	19.551	2810	2816	2823	rBV	1870175	2447665	83.41%	11.015%
52	19.622	2824	2828	2836	rVB	28404	48257	1.64%	0.217%
53	19.822	2859	2862	2866	rVB	21957	25145	0.86%	0.113%
54	20.980	3056	3059	3062	rBV2	26737	31310	1.07%	0.141%
55	21.233	3098	3102	3110	rVB	604331	824356	28.09%	3.710%
56	21.498	3140	3147	3158	rVB	767608	1376010	46.89%	6.192%
57	24.521	3651	3661	3674	rVB	1095033	2934453	100.00%	13.206%
58	24.739	3690	3698	3710	rBV	584449	1508104	51.39%	6.787%




Sum of corrected areas: 22221421

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022660.D
Acq On : 27 Oct 2024 03:30
Operator : RC/JU
Sample : P4559-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

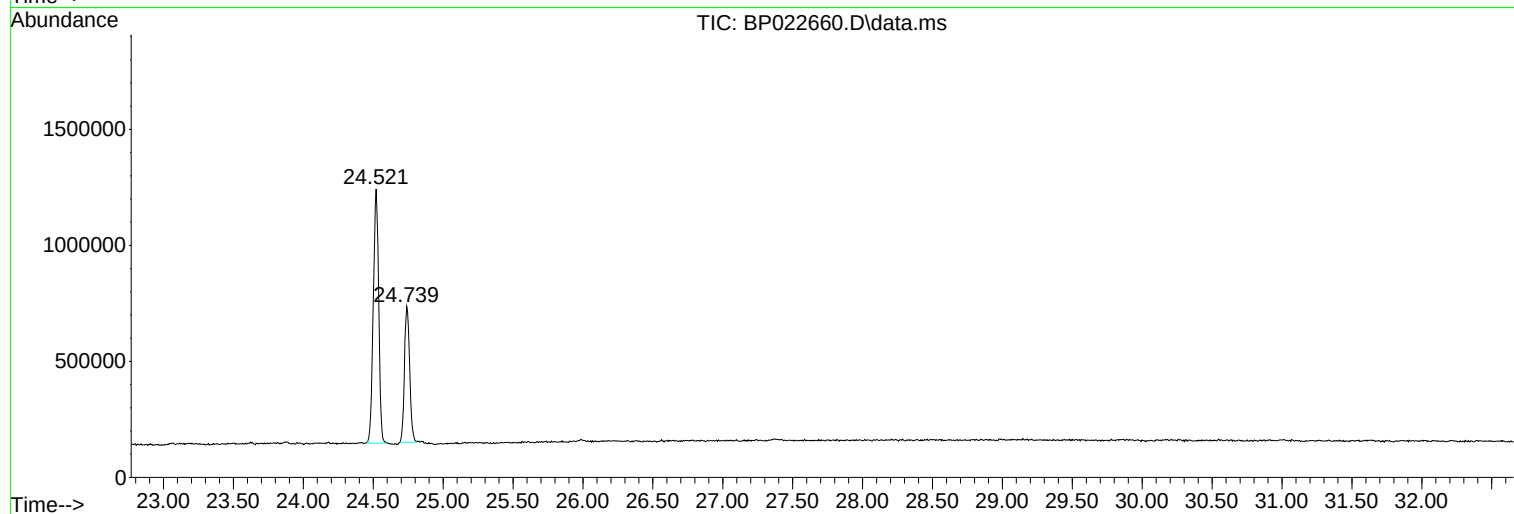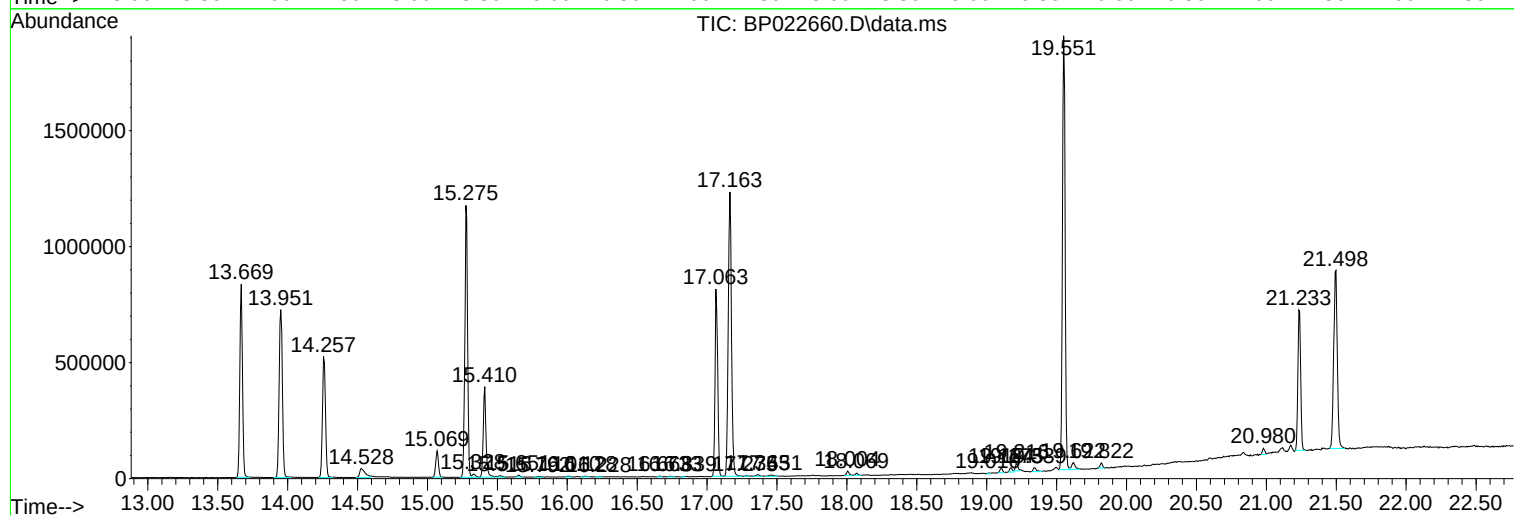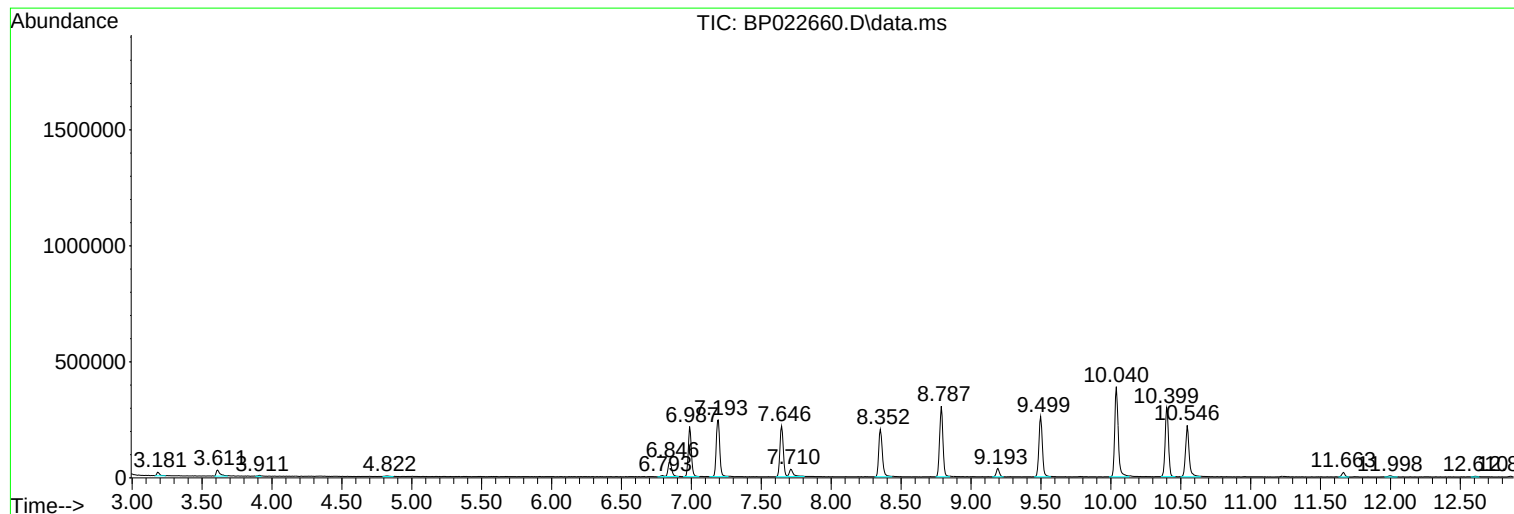

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022660.D
Acq On : 27 Oct 2024 03:30
Operator : RC/JU
Sample : P4559-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022660.D
Acq On : 27 Oct 2024 03:30
Operator : RC/JU
Sample : P4559-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------