

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022662.D
 Acq On : 27 Oct 2024 04:51
 Operator : RC/JU
 Sample : P4559-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	25	28	30	rBV2	4042	4854	0.16%	0.021%
2	3.181	30	33	42	rVB	17812	26141	0.86%	0.114%
3	3.605	101	105	117	rBV	46976	79933	2.63%	0.348%
4	3.911	154	157	163	rVB3	4210	6400	0.21%	0.028%
5	4.428	238	245	251	rBV	31308	44428	1.46%	0.193%
6	6.793	642	647	650	rBV	5355	7600	0.25%	0.033%
7	6.846	650	656	668	rVB	65789	120351	3.96%	0.524%
8	6.987	674	680	689	rBV	227403	365364	12.02%	1.591%
9	7.187	708	714	725	rBV	282688	454141	14.94%	1.977%
10	7.646	785	792	800	rBV	271936	436026	14.35%	1.899%
11	7.716	800	804	810	rVB4	6912	11110	0.37%	0.048%
12	8.352	905	912	928	rBV	219324	384803	12.66%	1.676%
13	8.787	979	986	998	rBV	316043	547909	18.03%	2.386%
14	9.193	1047	1055	1062	rBV2	34458	55384	1.82%	0.241%
15	9.505	1098	1108	1128	rBV	271066	495620	16.31%	2.158%
16	10.040	1191	1199	1225	rBV	377908	736681	24.24%	3.208%
17	10.399	1250	1260	1270	rBV	375815	606345	19.95%	2.640%
18	10.546	1278	1285	1304	rBV	310160	563129	18.53%	2.452%
19	11.228	1393	1401	1404	rBV7	2274	5009	0.16%	0.022%
20	11.669	1470	1476	1484	rVB2	17256	28516	0.94%	0.124%
21	11.999	1527	1532	1541	rBV3	5718	10612	0.35%	0.046%
22	12.863	1673	1679	1685	rVB10	2042	4043	0.13%	0.018%
23	13.675	1811	1817	1829	rBV	953972	1140798	37.54%	4.967%
24	13.787	1833	1836	1845	rVB9	1539	3565	0.12%	0.016%
25	13.957	1856	1865	1876	rBV2	758152	1249272	41.11%	5.440%
26	14.257	1909	1916	1930	rBV	541204	882964	29.05%	3.845%
27	14.522	1955	1961	1978	rBV3	30814	109396	3.60%	0.476%
28	15.075	2050	2055	2061	rVB	9305	12617	0.42%	0.055%
29	15.275	2081	2089	2098	rBV	1069618	1721887	56.66%	7.498%
30	15.416	2107	2113	2126	rBV	422216	560977	18.46%	2.443%
31	15.522	2127	2131	2134	rVB4	5549	8317	0.27%	0.036%
32	16.469	2285	2292	2296	rBV8	2516	6619	0.22%	0.029%
33	16.739	2336	2338	2343	rVB5	2252	3055	0.10%	0.013%
34	16.845	2352	2356	2362	rBV8	2024	3776	0.12%	0.016%
35	17.075	2388	2395	2404	rBV	926457	1194279	39.30%	5.200%
36	17.163	2404	2410	2426	rVB2	1445552	2075194	68.28%	9.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022662.D
Acq On : 27 Oct 2024 04:51
Operator : RC/JU
Sample : P4559-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	17.375	2443	2446	2449	rBV4	3101	4421	0.15%	0.019%
38	18.010	2550	2554	2560	rBV4	20700	30949	1.02%	0.135%
39	18.075	2563	2565	2568	rVB2	3656	3124	0.10%	0.014%
40	19.098	2735	2739	2743	rBV3	17396	23094	0.76%	0.101%
41	19.175	2748	2752	2755	rBV	23626	35929	1.18%	0.156%
42	19.204	2755	2757	2766	rVB5	39756	61288	2.02%	0.267%
43	19.339	2777	2780	2786	rVB4	16618	25105	0.83%	0.109%
44	19.492	2803	2806	2809	rBV5	7746	9312	0.31%	0.041%
45	19.551	2810	2816	2823	rBV	2228398	2650529	87.21%	11.541%
46	21.492	3140	3146	3157	rVB	970790	1512560	49.77%	6.586%
47	24.533	3653	3663	3677	rVB	1176289	3039149	100.00%	13.234%
48	24.745	3691	3699	3713	rVB	538437	1602943	52.74%	6.980%




Sum of corrected areas: 22965518

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022662.D
Acq On : 27 Oct 2024 04:51
Operator : RC/JU
Sample : P4559-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

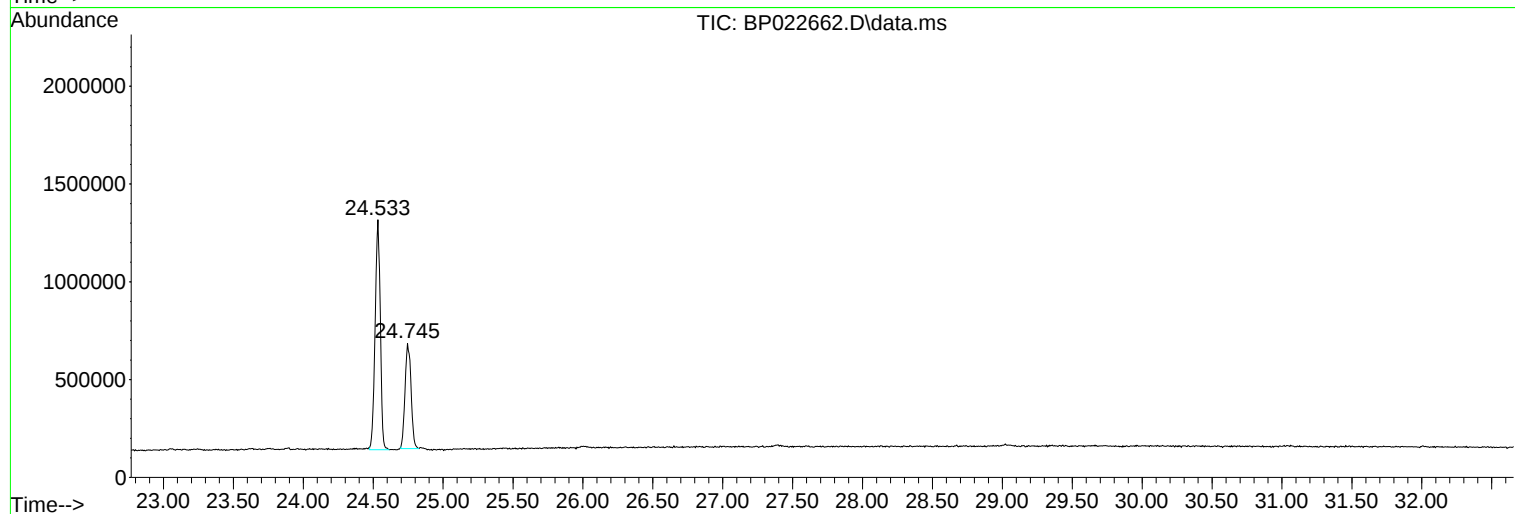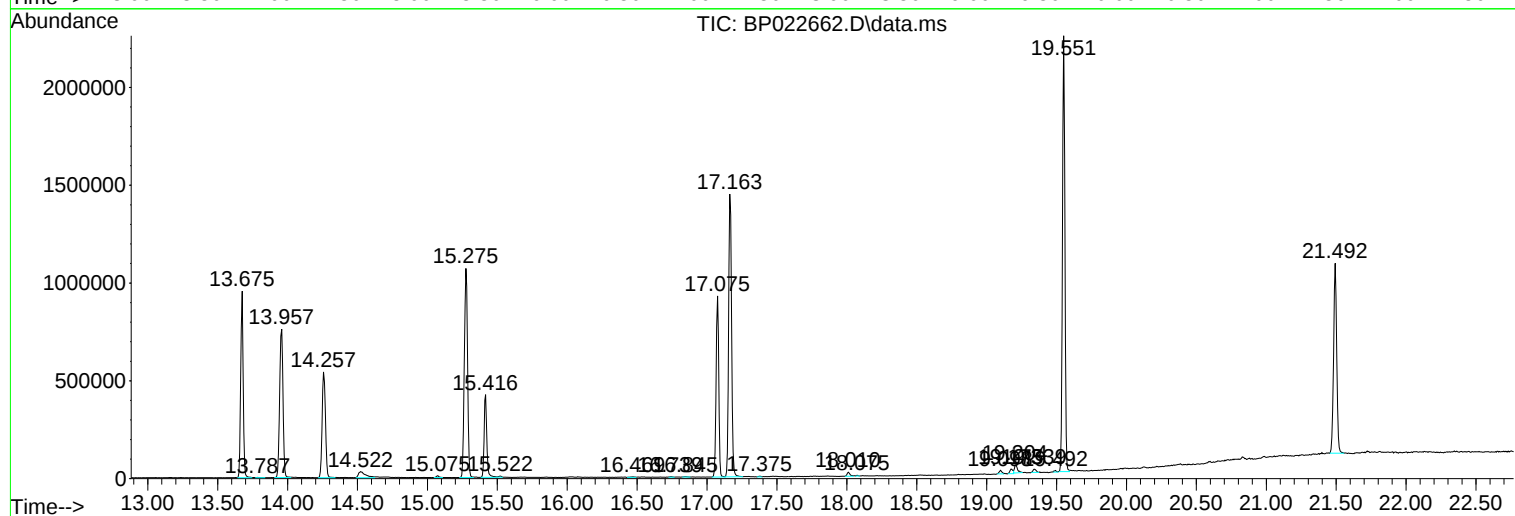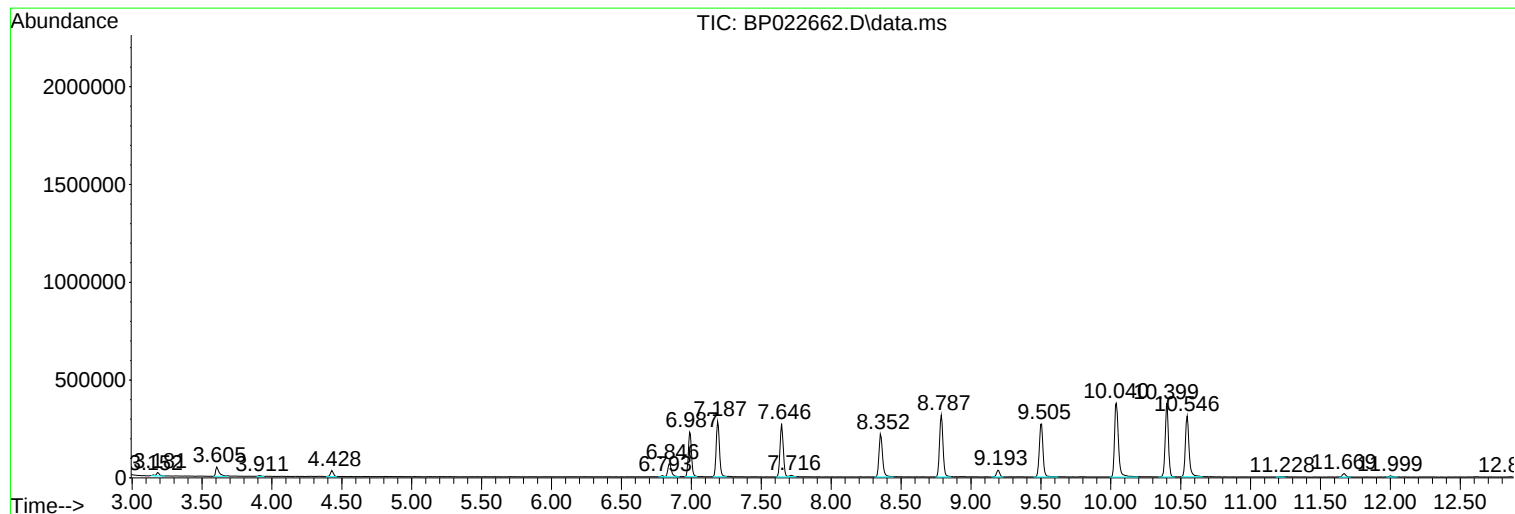

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022662.D
Acq On : 27 Oct 2024 04:51
Operator : RC/JU
Sample : P4559-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.428	2.04 ng/ul	44428	1,4-Dichlorobenzene-d4	7.646

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	93
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	27

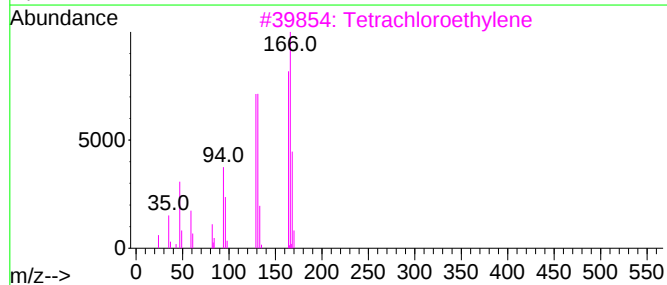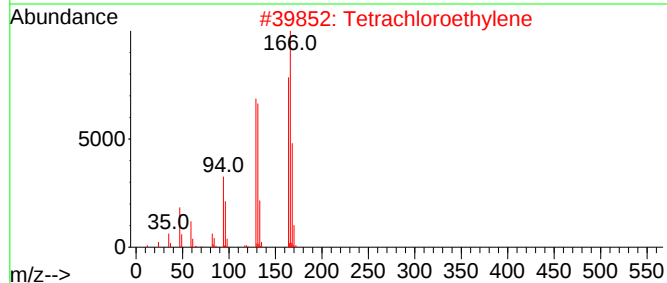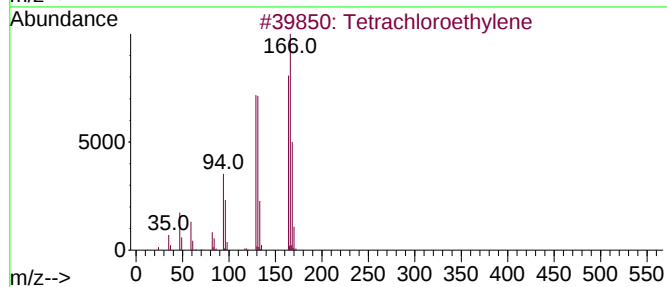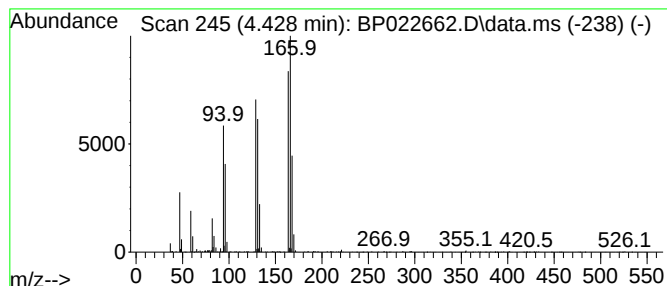

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022662.D
Acq On : 27 Oct 2024 04:51
Operator : RC/JU
Sample : P4559-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.428	2.0	ng/ul	44428	1	7.646	436026	20.0