

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022666.D
 Acq On : 27 Oct 2024 07:34
 Operator : RC/JU
 Sample : P4559-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	45	rVB	20234	28364	0.88%	0.107%
2	3.605	101	105	122	rBV	194009	311971	9.67%	1.180%
3	3.917	154	158	164	rVB3	3727	5616	0.17%	0.021%
4	4.834	308	314	322	rVB6	4603	8571	0.27%	0.032%
5	6.793	643	647	651	rBV2	12059	19176	0.59%	0.073%
6	6.846	651	656	672	rVB	99280	172958	5.36%	0.654%
7	6.993	674	681	696	rVV	293578	466772	14.47%	1.766%
8	7.193	708	715	726	rBV	336699	571948	17.73%	2.163%
9	7.646	785	792	804	rBV	303148	487796	15.12%	1.845%
10	8.358	906	913	926	rBV	284750	507273	15.73%	1.919%
11	8.793	979	987	1006	rBV	398583	678077	21.02%	2.565%
12	8.957	1010	1015	1021	rVB10	2067	4330	0.13%	0.016%
13	9.193	1048	1055	1062	rVB	55756	91330	2.83%	0.345%
14	9.499	1101	1107	1122	rBV	361027	593434	18.40%	2.245%
15	10.040	1192	1199	1219	rBV	494509	904350	28.04%	3.421%
16	10.404	1253	1261	1273	rBV	403473	670728	20.79%	2.537%
17	10.546	1277	1285	1303	rBV	459961	830518	25.75%	3.141%
18	10.775	1318	1324	1332	rVB5	3892	7265	0.23%	0.027%
19	11.669	1470	1476	1482	rVB	17628	26245	0.81%	0.099%
20	12.010	1528	1534	1541	rBV3	6369	12463	0.39%	0.047%
21	12.251	1569	1575	1579	rBV6	2040	3537	0.11%	0.013%
22	12.881	1679	1682	1687	rVB3	3293	4744	0.15%	0.018%
23	13.222	1737	1740	1748	rBV9	1870	4788	0.15%	0.018%
24	13.675	1809	1817	1828	rBV	949718	1420651	44.04%	5.374%
25	13.951	1856	1864	1879	rBV	1039898	1579401	48.96%	5.974%
26	14.263	1910	1917	1930	rVB	653642	996854	30.90%	3.771%
27	14.534	1957	1963	1966	rBV4	12704	23742	0.74%	0.090%
28	14.563	1966	1968	1978	rVB6	9052	17852	0.55%	0.068%
29	14.716	1986	1994	2004	rVB6	4468	13864	0.43%	0.052%
30	15.081	2050	2056	2062	rBV	34075	41892	1.30%	0.158%
31	15.269	2081	2088	2102	rBV	1403939	2134464	66.17%	8.074%
32	15.422	2108	2114	2124	rBV2	76914	127775	3.96%	0.483%
33	15.516	2126	2130	2136	rVB5	6101	10976	0.34%	0.042%
34	15.645	2146	2152	2162	rBV	32894	55140	1.71%	0.209%
35	16.069	2222	2224	2231	rVB8	2429	4565	0.14%	0.017%
36	16.216	2244	2249	2254	rBV3	8970	13677	0.42%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
 Data File : BP022666.D
 Acq On : 27 Oct 2024 07:34
 Operator : RC/JU
 Sample : P4559-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCNY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	16.475	2286	2293	2298	rBV9	3298	7369	0.23%	0.028%
38	16.539	2300	2304	2309	rVB8	2608	4475	0.14%	0.017%
39	16.745	2333	2339	2342	rBV8	1790	3322	0.10%	0.013%
40	17.063	2385	2393	2403	rBV	791471	1314497	40.75%	4.972%
41	17.169	2404	2411	2425	rVV	1982384	2555916	79.23%	9.668%
42	17.275	2425	2429	2437	rVB8	10638	19891	0.62%	0.075%
43	17.998	2546	2552	2560	rBV7	16449	34651	1.07%	0.131%
44	18.069	2562	2564	2571	rVB5	3220	5785	0.18%	0.022%
45	18.298	2599	2603	2607	rBV7	3769	7478	0.23%	0.028%
46	18.675	2665	2667	2671	rBV4	2484	3358	0.10%	0.013%
47	19.081	2732	2736	2741	rBV3	23474	32844	1.02%	0.124%
48	19.163	2746	2750	2754	rVV	19152	31776	0.99%	0.120%
49	19.204	2754	2757	2767	rVB2	60541	92218	2.86%	0.349%
50	19.333	2776	2779	2785	rBV6	12231	22058	0.68%	0.083%
51	19.486	2803	2805	2808	rVB3	9084	8554	0.27%	0.032%
52	19.545	2808	2815	2823	rBV	2022205	3035683	94.11%	11.482%
53	20.128	2911	2914	2917	rBV3	16684	19293	0.60%	0.073%
54	21.510	3143	3149	3156	rBV2	994332	1538136	47.68%	5.818%
55	24.527	3653	3662	3674	rVB	1136381	3225777	100.00%	12.201%
56	24.763	3694	3702	3713	rVB	693994	1621626	50.27%	6.134%




Sum of corrected areas: 26437814

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022666.D
Acq On : 27 Oct 2024 07:34
Operator : RC/JU
Sample : P4559-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

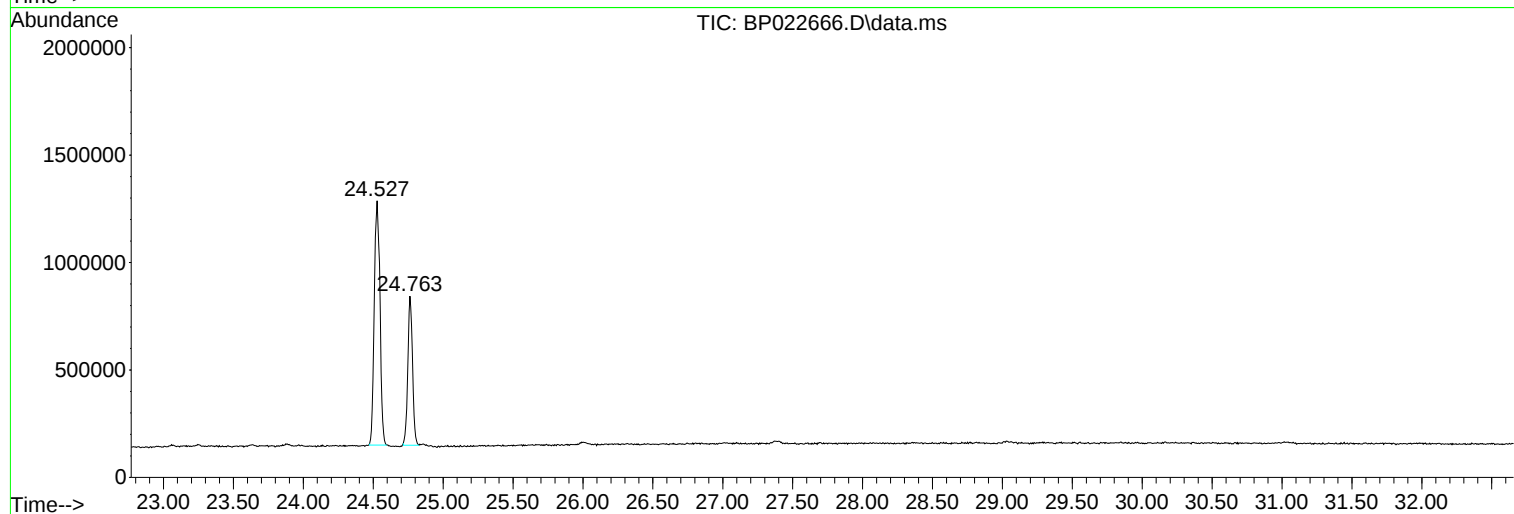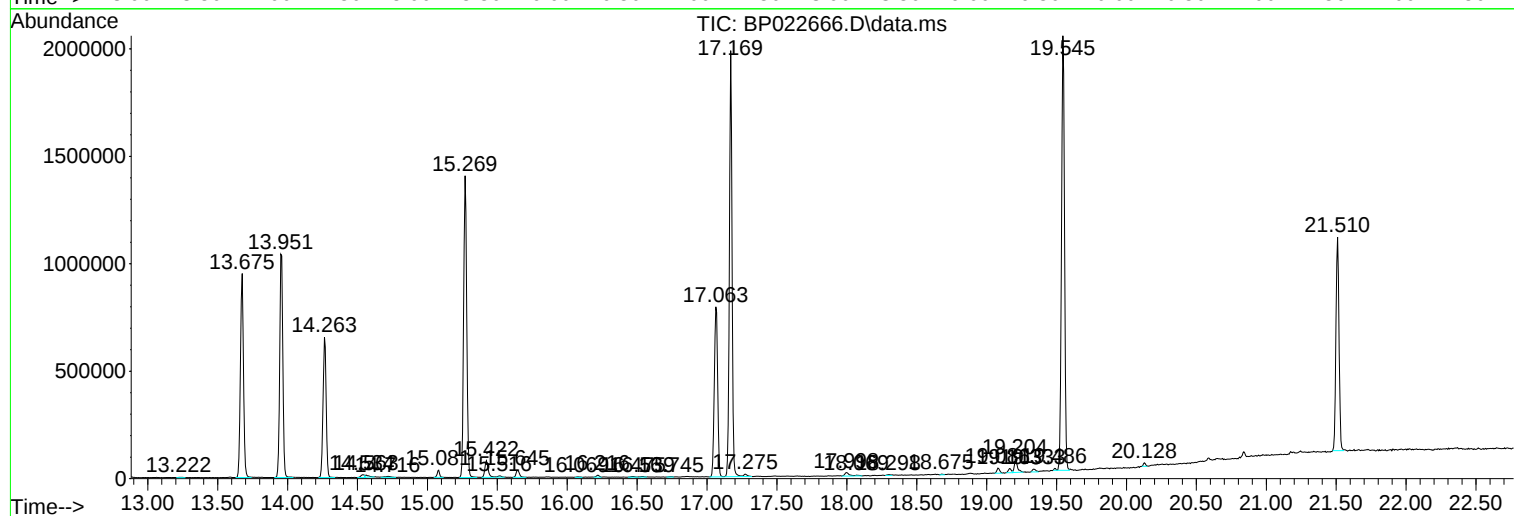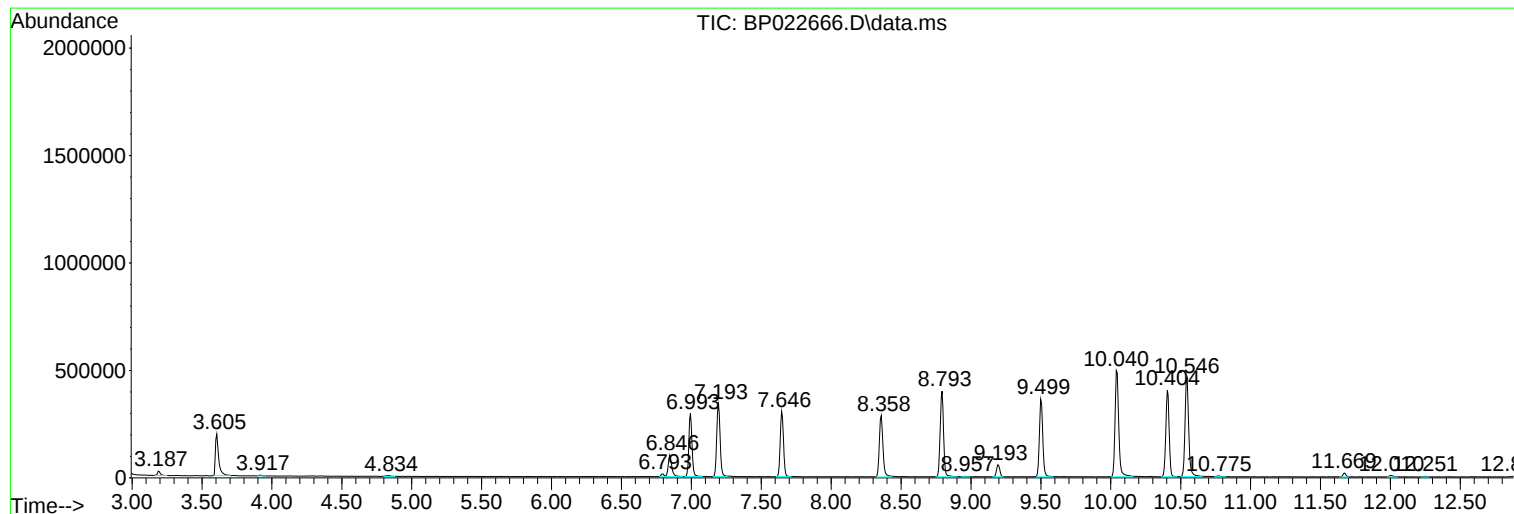

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022666.D
Acq On : 27 Oct 2024 07:34
Operator : RC/JU
Sample : P4559-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY6









Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.193	2.72 ng/ul	91330	Naphthalene-d8	10.405

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	91
2			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	91
3			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	90
4			(E)-N-[2-Hydroxy-2-(4-hydroxyphe...	515	C26H41NO4Si3	1010480-65-8	53
5			Methyl 4-hydroxymandelatem, 2TMS...	326	C15H26O4Si2	055334-40-2	50

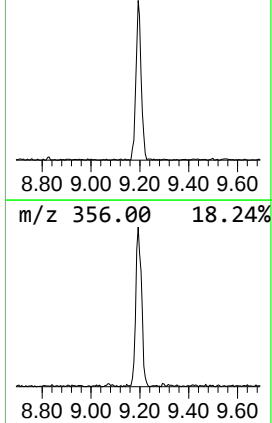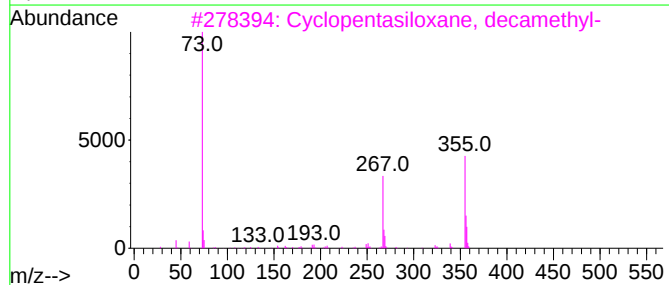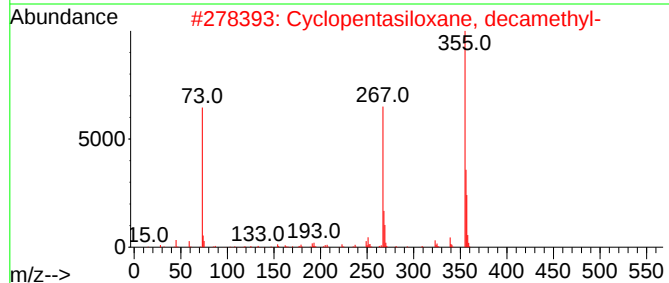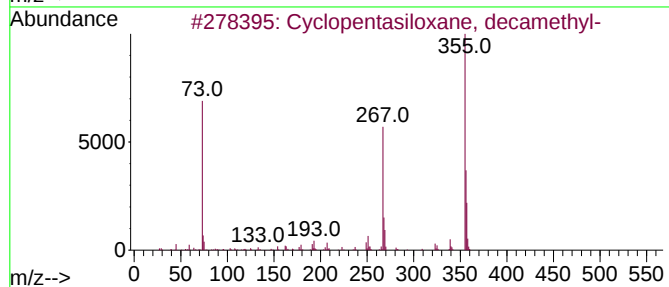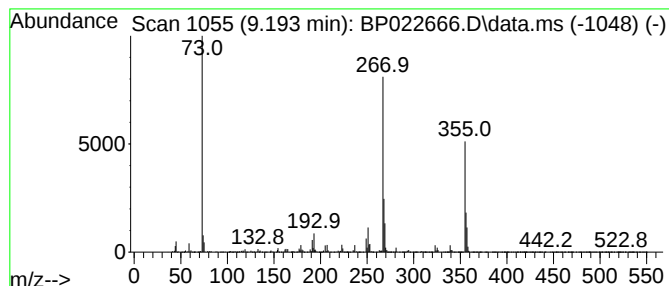

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102524\
Data File : BP022666.D
Acq On : 27 Oct 2024 07:34
Operator : RC/JU
Sample : P4559-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCNY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasilox...	9.193	2.7	ng/ul	91330	2	10.405	670728	20.0