

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102622\
 Data File : BP012331.D
 Acq On : 26 Oct 2022 16:23
 Operator : CG/JU
 Sample : N5070-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBL1

Quant Time: Oct 27 00:24:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	316413	20.000	ng/ul	0.00
20) Naphthalene-d8	10.616	136	1504408	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	1019498	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.222	188	2305211	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	2572249	20.000	ng/ul	0.00
88) Perylene-d12	23.710	264	2892518	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	20691	2.633	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.981	99	384637	13.553	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	271743	16.040	ng/ul	0.00
11) 2-Chlorophenol-d4	7.346	132	321341	15.505	ng/ul	0.00
15) 4-Methylphenol-d8	8.528	113	164068	7.310	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	168233	17.244	ng/ul	0.00
24) 2-Nitrophenol-d4	9.699	143	182041	17.978	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.240	165	341776	15.575	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	292974	8.966	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	1235382	17.701	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	1391604	17.448	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	144383	10.931	ng/ul	0.00
60) Fluorene-d10	15.457	176	1132604	18.955	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.587	200	119929	9.992	ng/ul	0.00
73) Anthracene-d10	17.316	188	1710979	17.226	ng/ul	0.00
81) Pyrene-d10	19.557	212	2368535	18.340	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.557	264	2628678	18.599	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.011	94	31274	1.060	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102622\
Data File : BP012331.D
Acq On : 26 Oct 2022 16:23
Operator : CG/JU
Sample : N5070-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BL1

Quant Time: Oct 27 00:24:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration

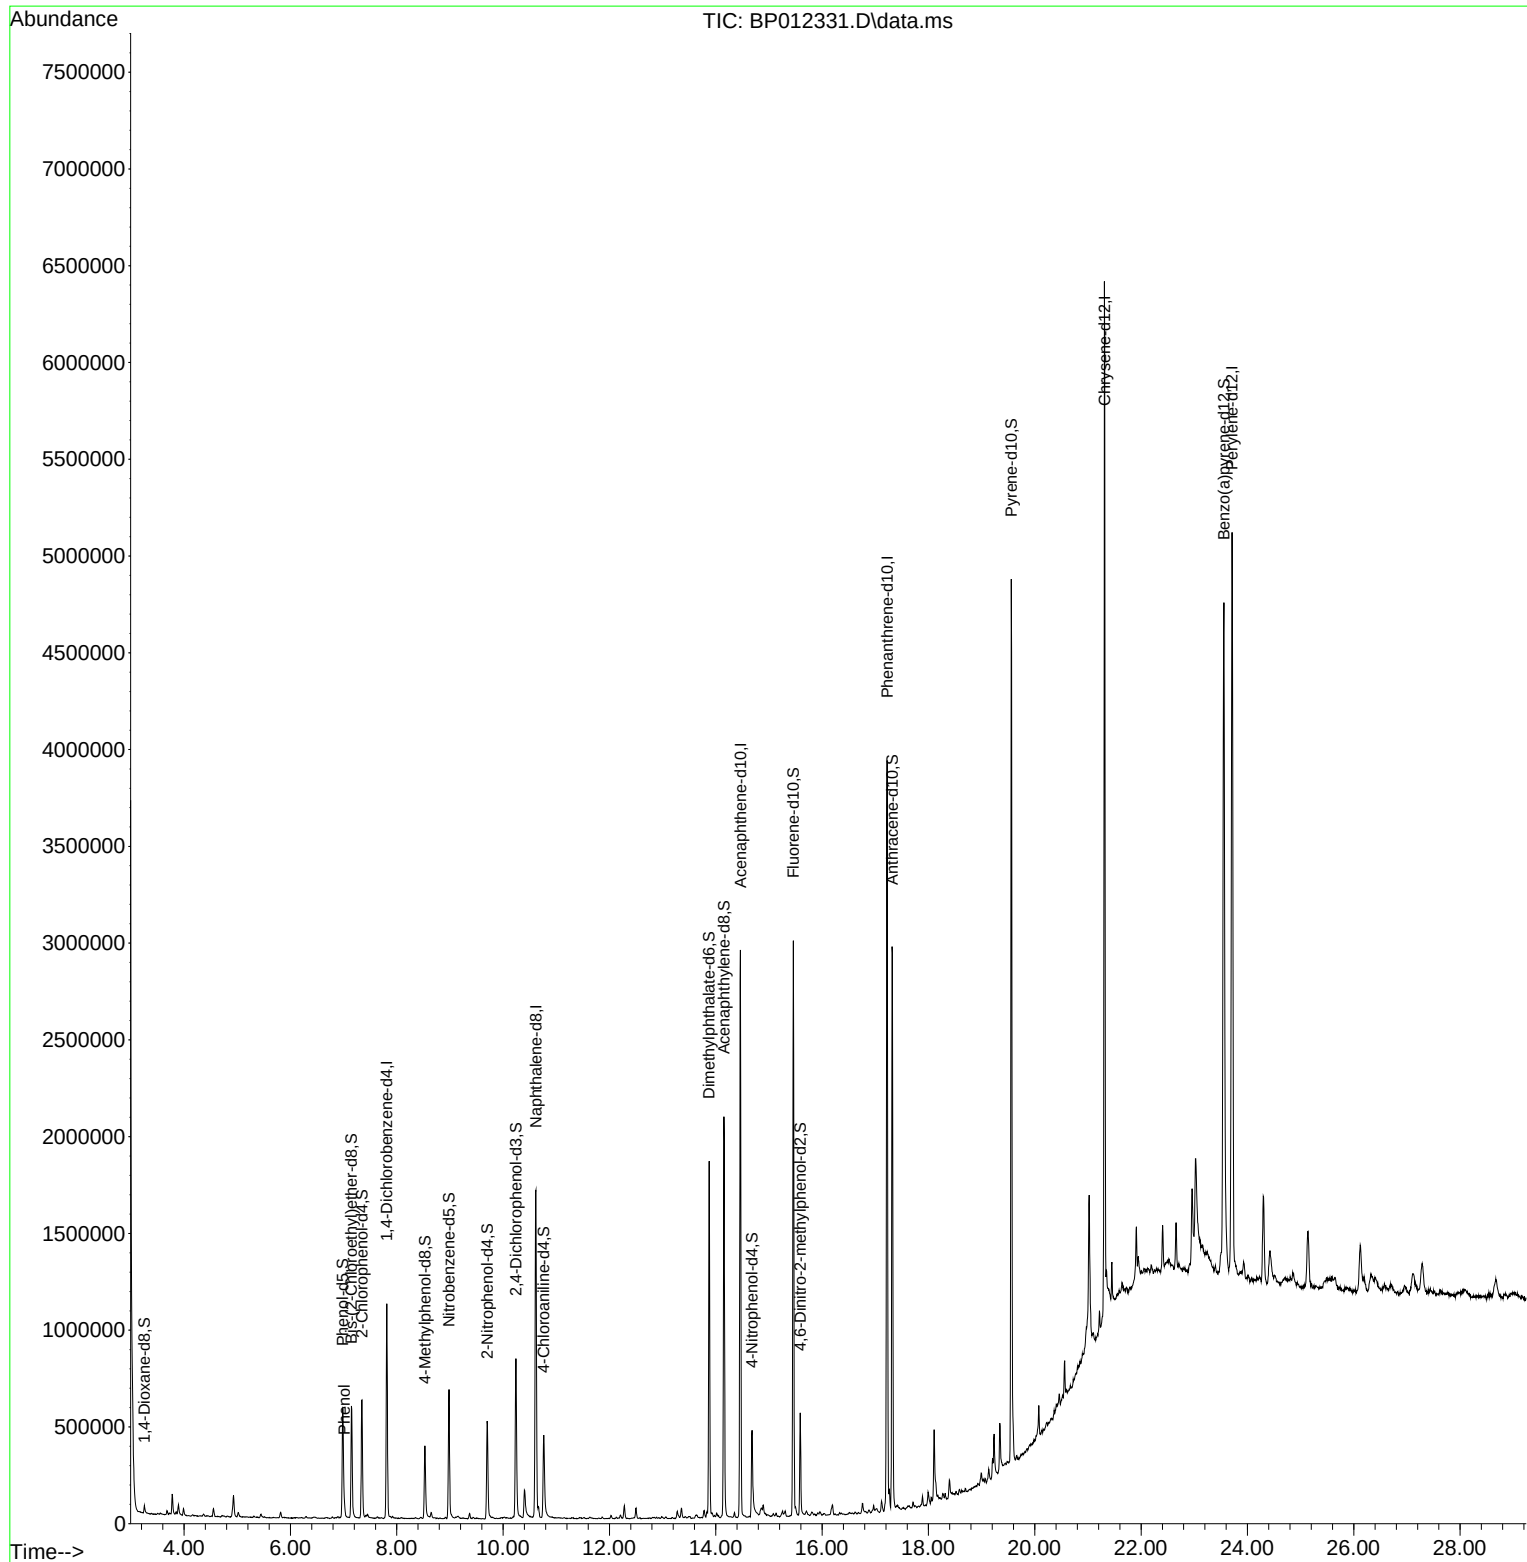

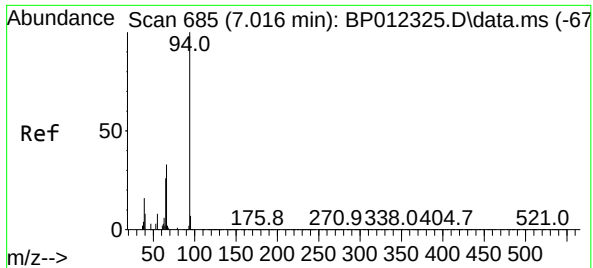

#8
Phenol
Concen: 1.060 ng/ul
RT: 7.011 min Scan# 61
Delta R.T. 0.001 min
Lab File: BP012331.D
Acq: 26 Oct 2022 16:23

Instrument :
BNA_P
ClientSampleId :
C0BL1

Tgt Ion: 94	Resp: 31274
Ion Ratio	Lower Upper
94 100	
65 25.9	20.8 31.2
66 38.5	26.2 39.2

