

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102622\
 Data File : BP012332.D
 Acq On : 26 Oct 2022 16:58
 Operator : CG/JU
 Sample : N5015-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BE7

Quant Time: Oct 27 00:25:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	297121	20.000	ng/ul	0.00
20) Naphthalene-d8	10.616	136	1392111	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	935498	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.222	188	2091554	20.000	ng/ul	0.00
79) Chrysene-d12	21.316	240	2322962	20.000	ng/ul	0.00
88) Perylene-d12	23.710	264	2752370	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	38048	5.156	ng/uL	0.00
4) Pyridine-d5	3.675	84	511152	24.114	ng/ul	0.00
7) Phenol-d5	6.981	99	784101	29.423	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	482174	30.308	ng/ul	0.00
11) 2-Chlorophenol-d4	7.346	132	612511	31.474	ng/ul	0.00
15) 4-Methylphenol-d8	8.528	113	656889	31.166	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	309596	34.295	ng/ul	0.00
24) 2-Nitrophenol-d4	9.705	143	339944	36.280	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.240	165	642063	31.619	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	947205	31.328	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	2138861	33.399	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	2402575	32.829	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	329213	27.162	ng/ul	0.00
60) Fluorene-d10	15.457	176	1861718	33.955	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.587	200	243354	22.348	ng/ul	0.00
73) Anthracene-d10	17.322	188	2968935	32.944	ng/ul	0.00
81) Pyrene-d10	19.563	212	3667413	31.445	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.557	264	4449930	33.089	ng/ul	0.00


Target Compounds					Qvalue	
8) Phenol	7.011	94	30346	1.095	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102622\
Data File : BP012332.D
Acq On : 26 Oct 2022 16:58
Operator : CG/JU
Sample : N5015-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BE7

Quant Time: Oct 27 00:25:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration

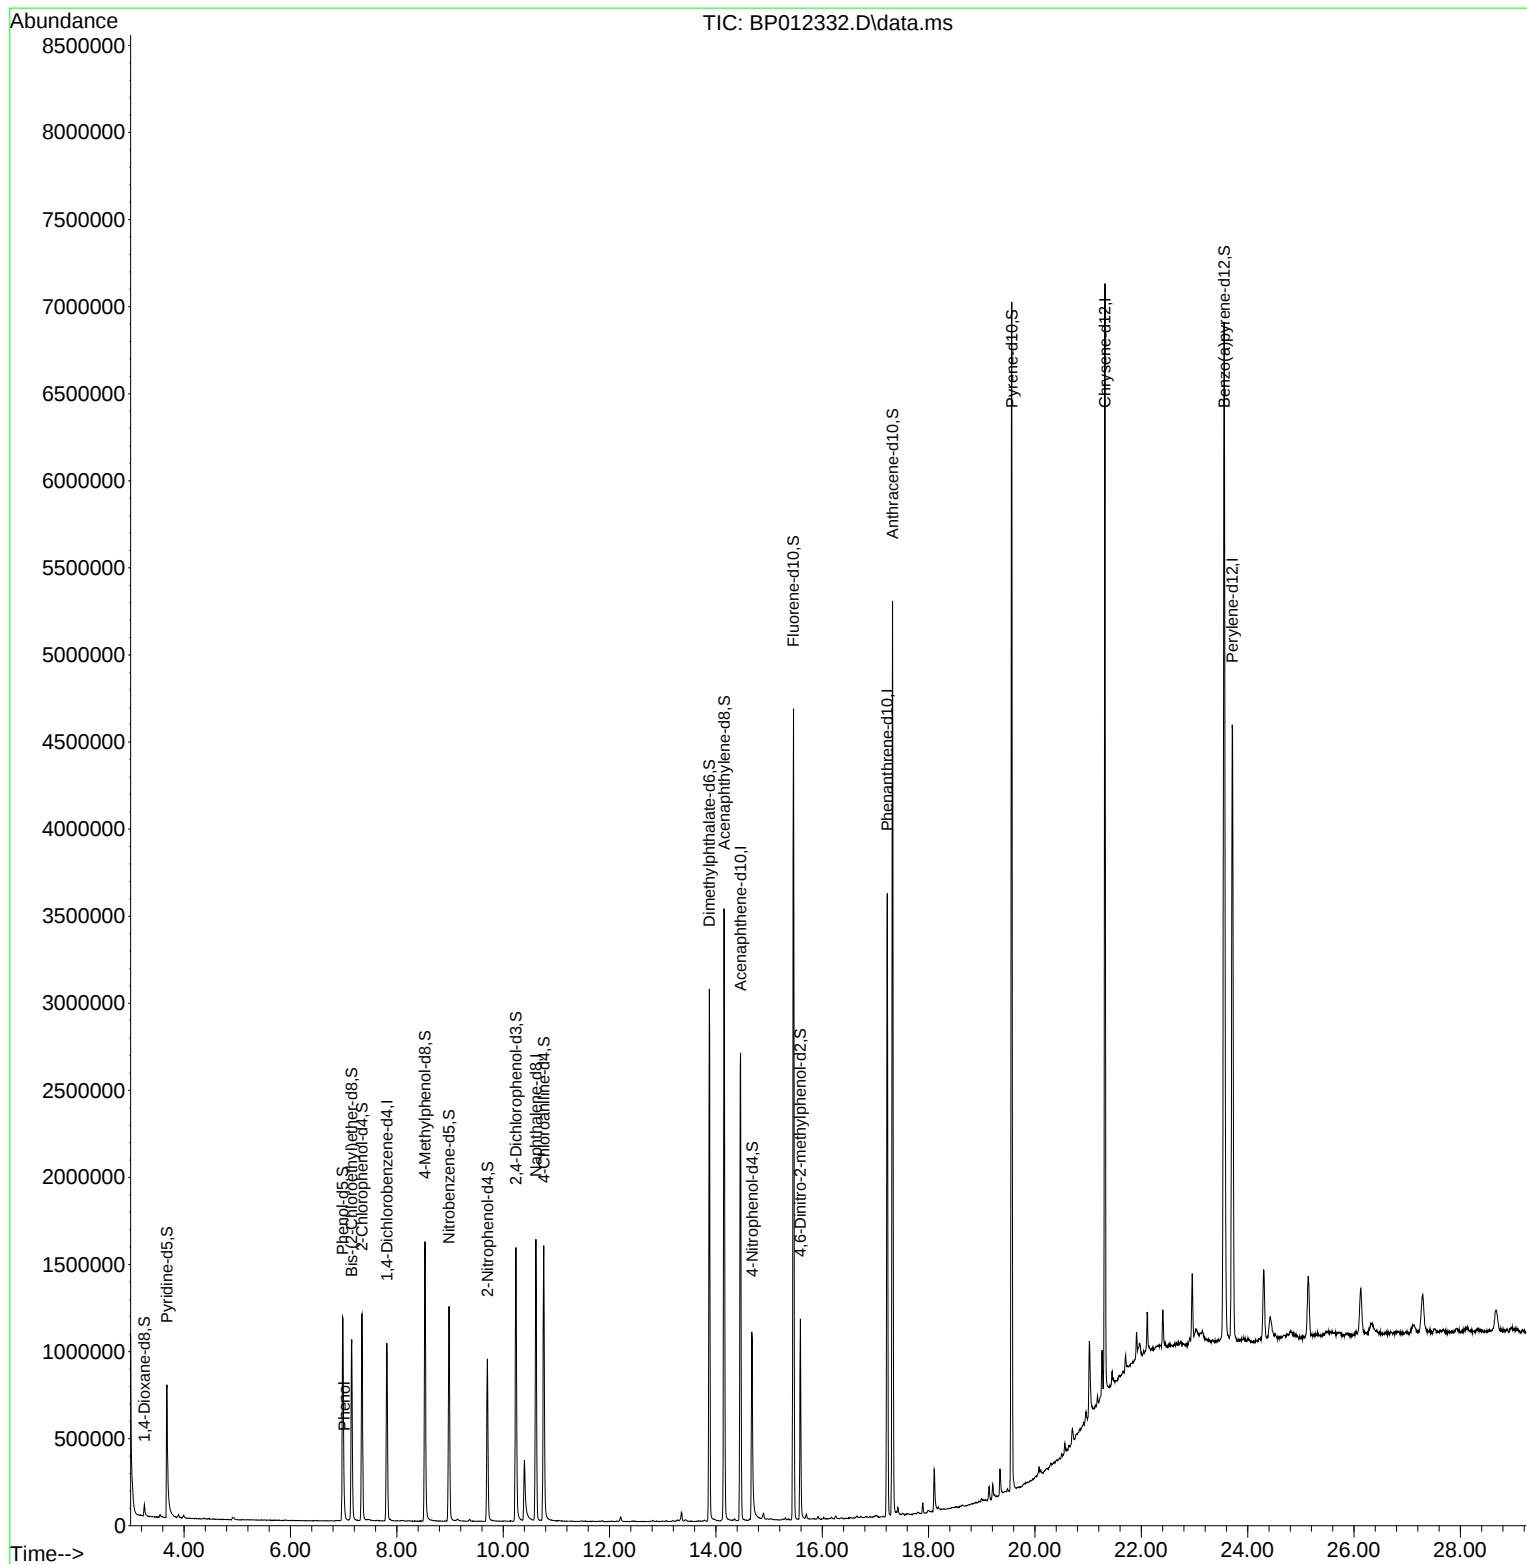

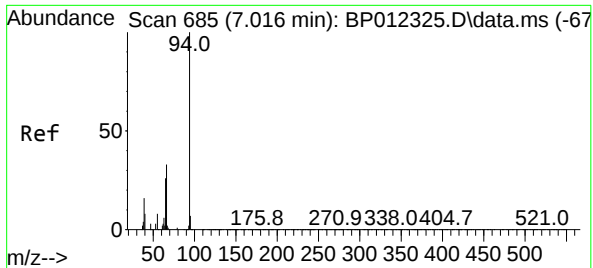

#8
Phenol
Concen: 1.095 ng/ul
RT: 7.011 min Scan# 61
Delta R.T. 0.001 min
Lab File: BP012332.D
Acq: 26 Oct 2022 16:58

Instrument :
BNA_P
ClientSampleId :
C1BE7

Tgt Ion: 94 Resp: 30346
Ion Ratio Lower Upper
94 100
65 27.0 20.8 31.2
66 40.4 26.2 39.2#

