
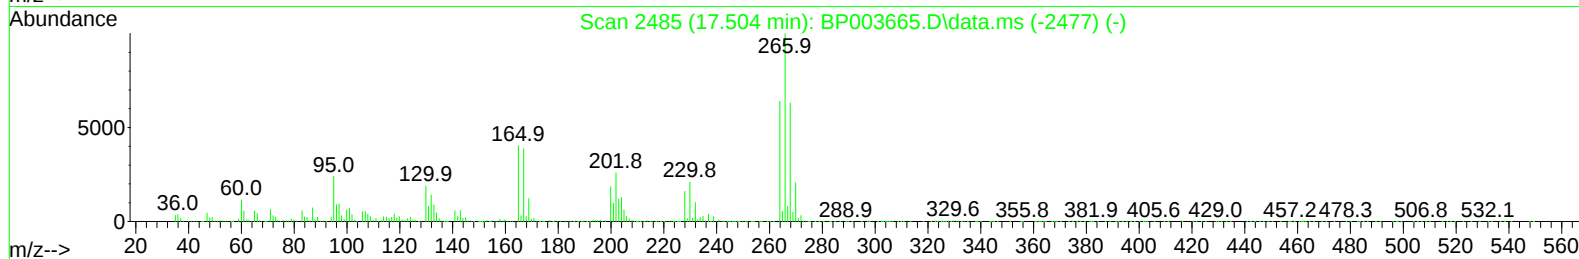
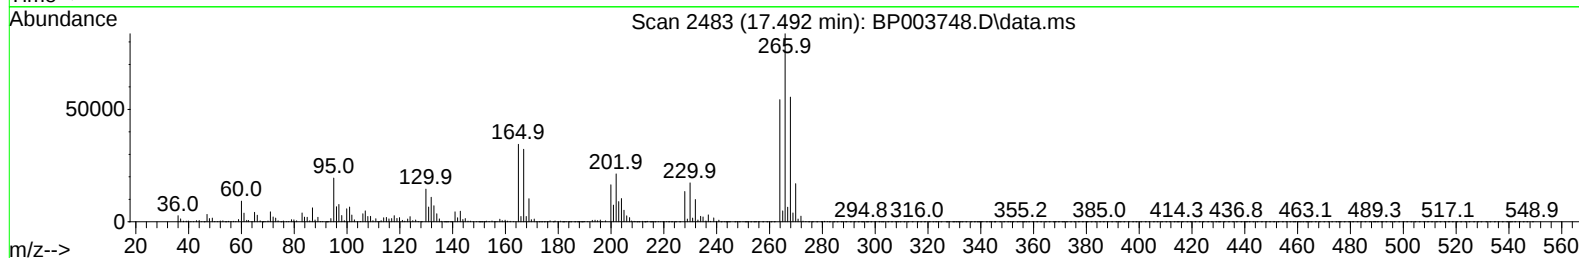


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102720\
Data File : BP003748.D
Acq On : 27 Oct 2020 10:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 02:18:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 16:22:21 2020
Response via : Initial Calibration

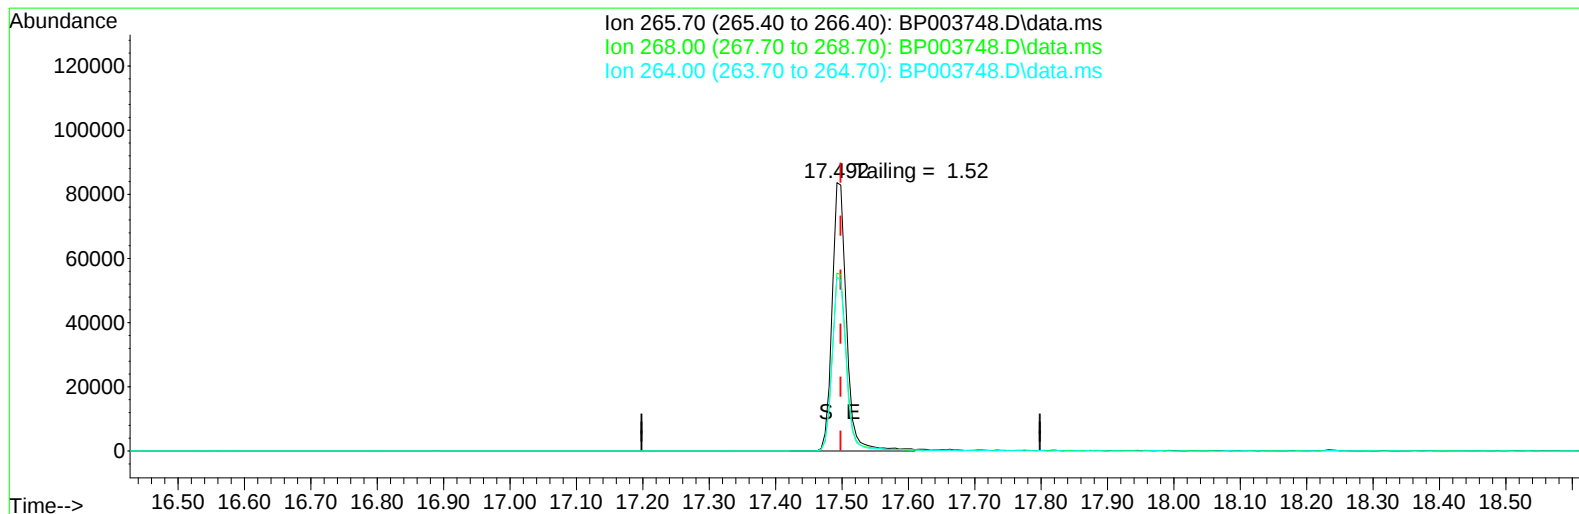

TIC: BP003748.D\data.ms

(70) Pentachlorophenol (C)




17.492min (-0.006) 77021.28 ng

response 126008

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	66.34
264.00	63.30	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102720\
Data File : BP003748.D
Acq On : 27 Oct 2020 10:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 02:18:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 16:22:21 2020
Response via : Initial Calibration

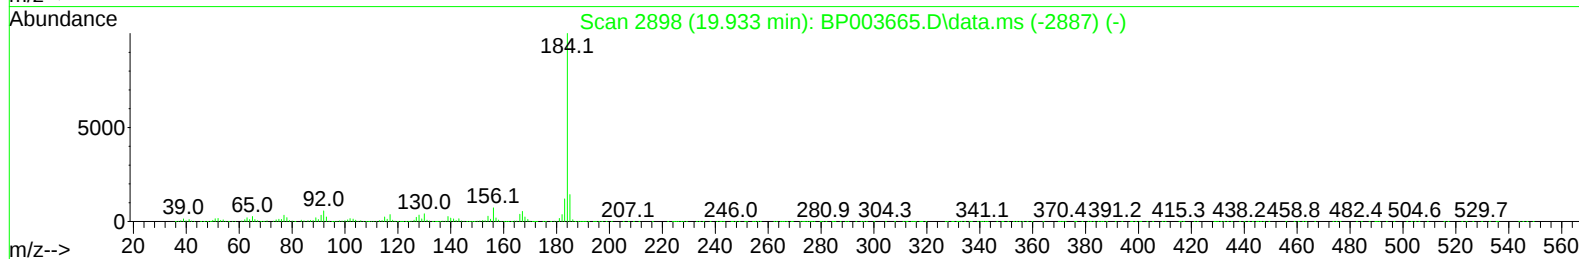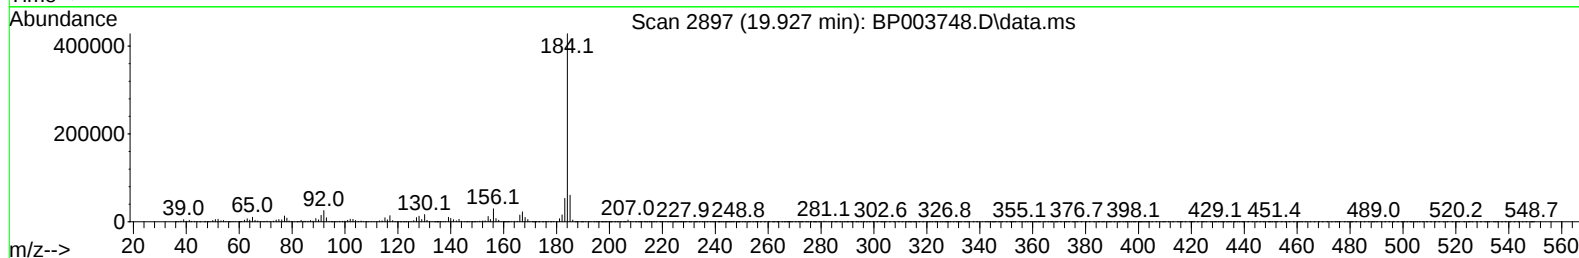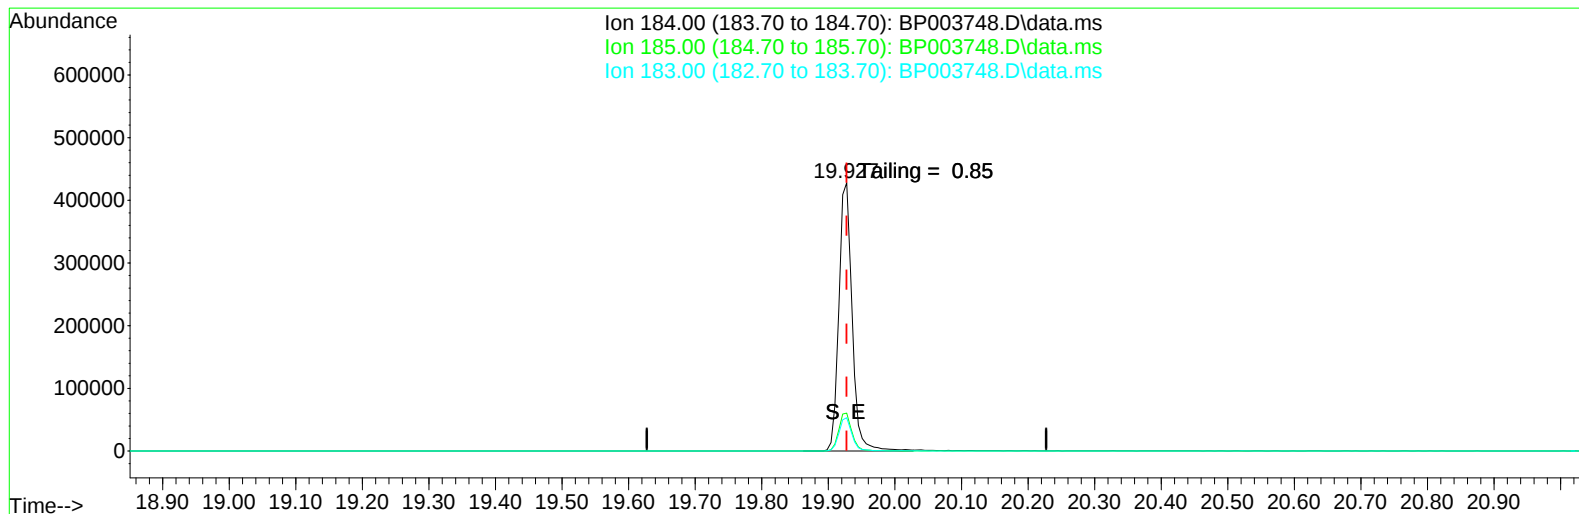

TIC: BP003748.D\data.ms

(77) Benzidine**19.927min (+ 0.000) 31169.68 ng****response 591490**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	12.00	12.40
0.00	0.00	0.00