

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP102720\  
 Data File : BP003760.D  
 Acq On : 27 Oct 2020 18:13  
 Operator : CG/JU  
 Sample : L4516-04  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 FRAC-TANK-2

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP101920.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003760.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.252       | 54            | 62          | 73           | rBV      | 216394         | 479367        | 3.50%           | 0.926%        |
| 2         | 3.346       | 73            | 78          | 84           | rBV      | 767672         | 1070249       | 7.80%           | 2.068%        |
| 3         | 6.011       | 521           | 531         | 539          | rBV      | 1268310        | 1939224       | 14.14%          | 3.748%        |
| 4         | 7.657       | 803           | 811         | 823          | rBV      | 721129         | 1183671       | 8.63%           | 2.288%        |
| 5         | 8.510       | 945           | 956         | 963          | rBV      | 655676         | 1050477       | 7.66%           | 2.030%        |
| 6         | 9.681       | 1145          | 1155        | 1163         | rBV      | 2151691        | 3713182       | 27.07%          | 7.176%        |
| 7         | 11.351      | 1432          | 1439        | 1452         | rVB      | 805807         | 1386082       | 10.11%          | 2.679%        |
| 8         | 13.740      | 1837          | 1845        | 1854         | rBV      | 6173124        | 8809332       | 64.23%          | 17.025%       |
| 9         | 14.528      | 1973          | 1979        | 1985         | rBV      | 255367         | 342613        | 2.50%           | 0.662%        |
| 10        | 15.110      | 2071          | 2078        | 2086         | rVB      | 1357738        | 1964543       | 14.32%          | 3.797%        |
| 11        | 16.586      | 2321          | 2329        | 2350         | rBV      | 5035602        | 7046809       | 51.38%          | 13.619%       |
| 12        | 17.828      | 2534          | 2540        | 2550         | rBV      | 1691253        | 2453971       | 17.89%          | 4.743%        |
| 13        | 18.645      | 2674          | 2679        | 2686         | rBV      | 173886         | 253513        | 1.85%           | 0.490%        |
| 14        | 20.304      | 2955          | 2961        | 2966         | rBV      | 11326787       | 13715038      | 100.00%         | 26.507%       |
| 15        | 21.474      | 3155          | 3160        | 3170         | rBV      | 851895         | 1057367       | 7.71%           | 2.044%        |
| 16        | 21.845      | 3218          | 3223        | 3230         | rVB      | 2037013        | 2708159       | 19.75%          | 5.234%        |
| 17        | 24.427      | 3653          | 3662        | 3671         | rBV2     | 1125779        | 2409575       | 17.57%          | 4.657%        |
| 18        | 25.033      | 3761          | 3765        | 3777         | rVB3     | 71547          | 158915        | 1.16%           | 0.307%        |




Sum of corrected areas: 51742087

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP102720\  
Data File : BP003760.D  
Acq On : 27 Oct 2020 18:13  
Operator : CG/JU  
Sample : L4516-04  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
FRAC-TANK-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP101920.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

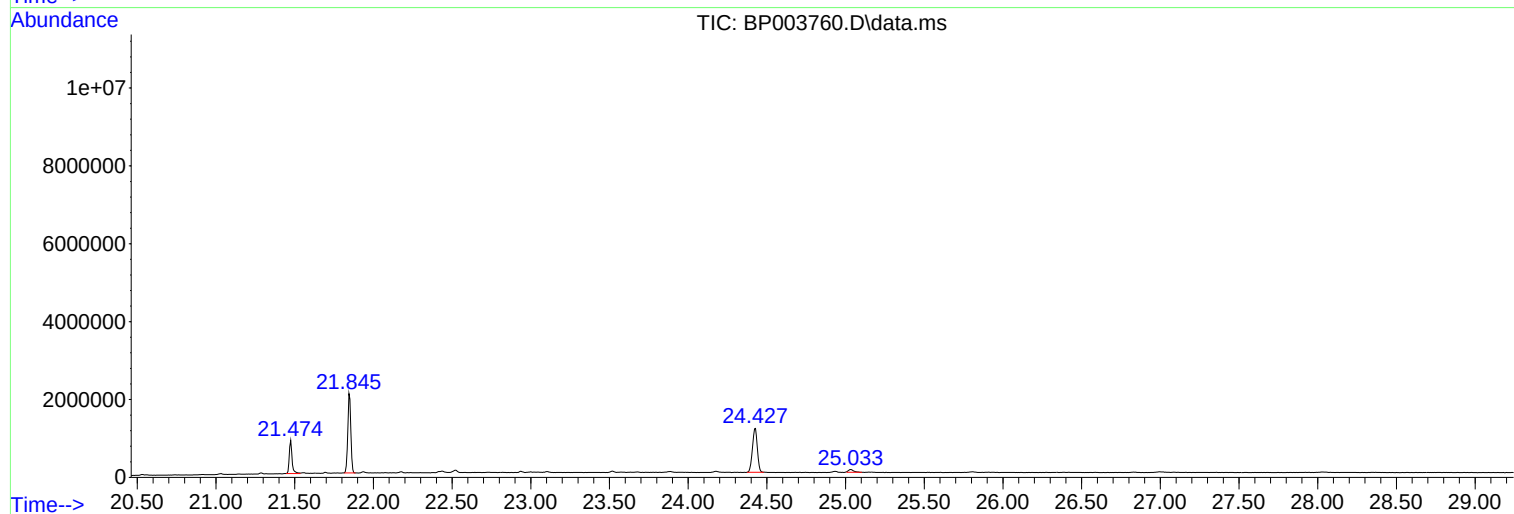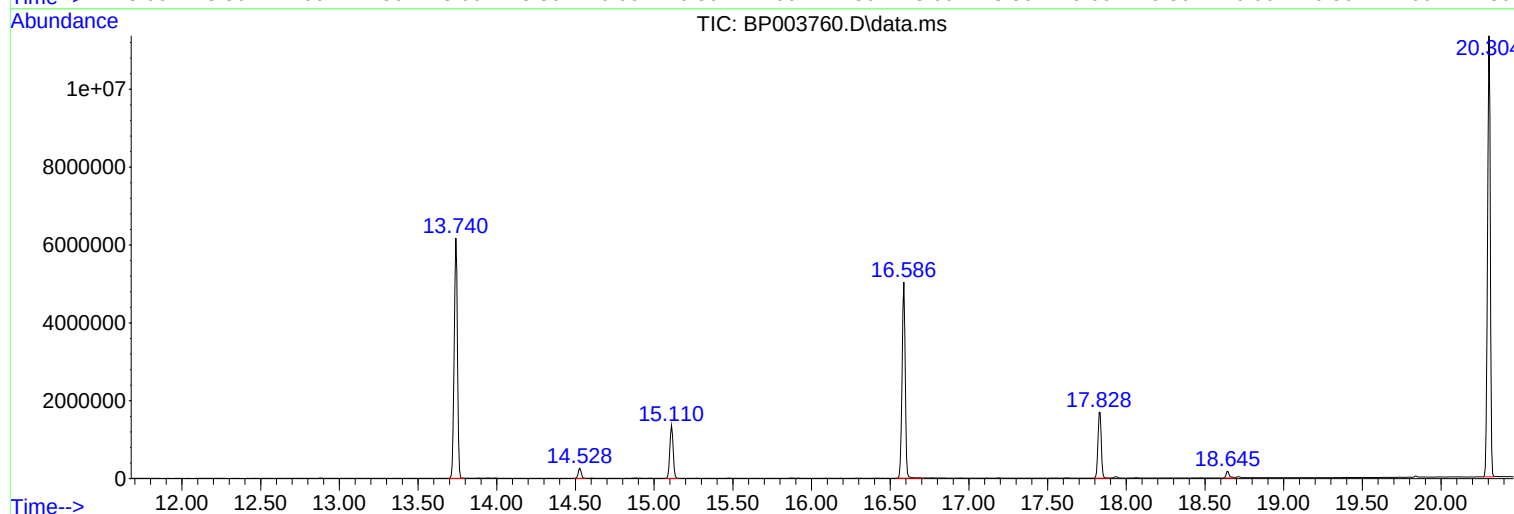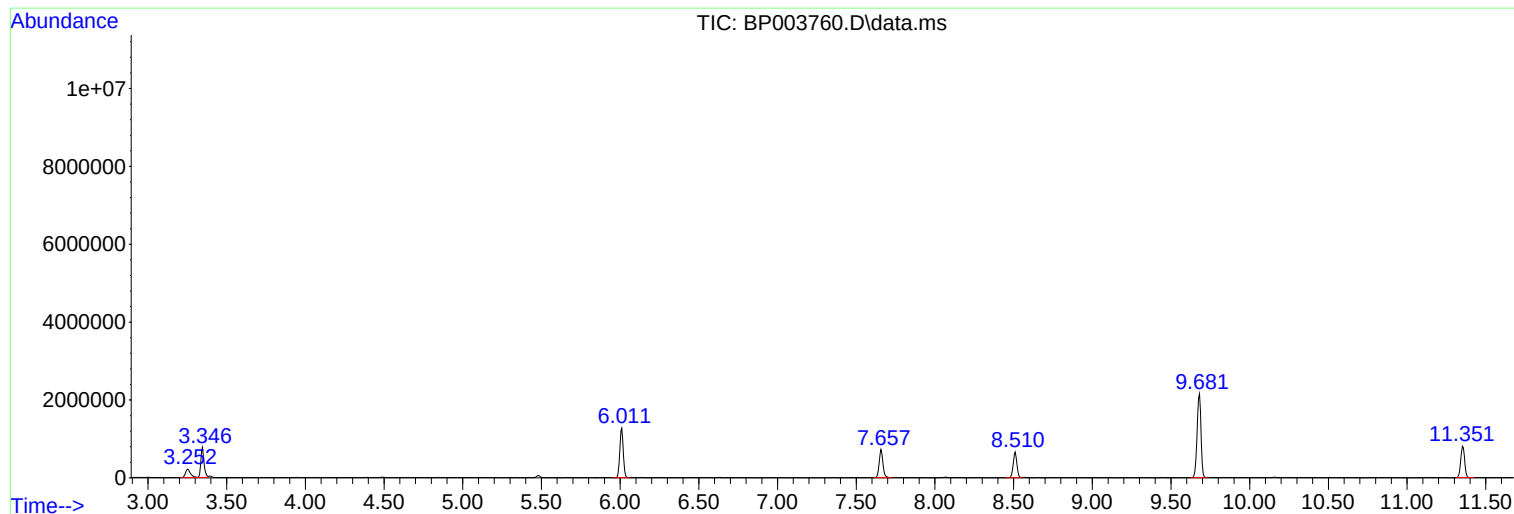

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP102720\  
Data File : BP003760.D  
Acq On : 27 Oct 2020 18:13  
Operator : CG/JU  
Sample : L4516-04  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
FRAC-TANK-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP101920.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP102720\  
Data File : BP003760.D  
Acq On : 27 Oct 2020 18:13  
Operator : CG/JU  
Sample : L4516-04  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
FRAC-TANK-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP101920.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----