
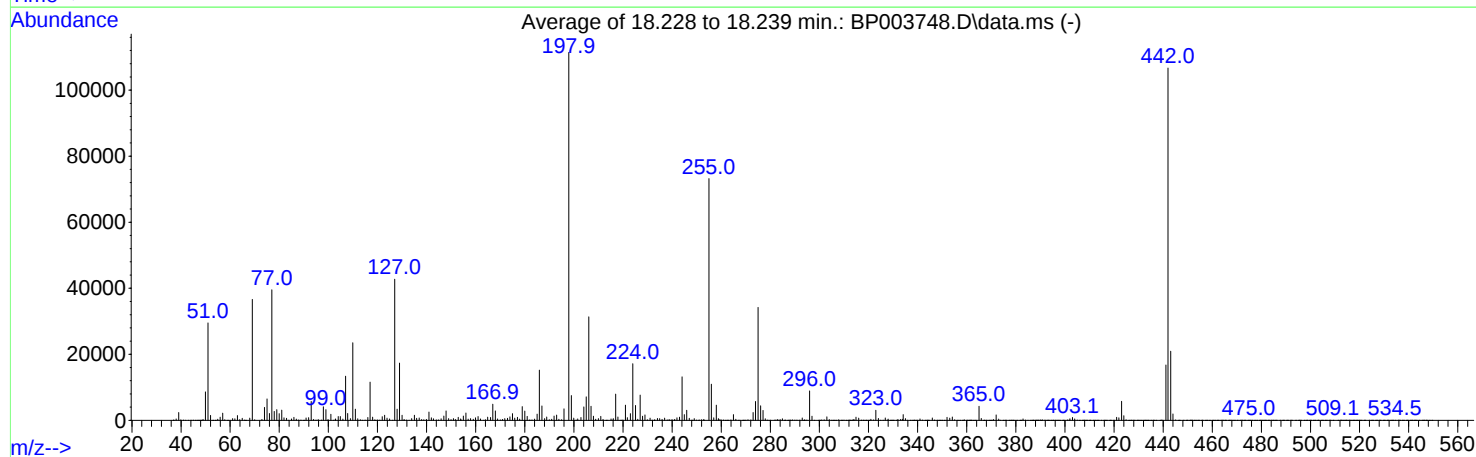


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102720\
 Data File : BP003748.D
 Acq On : 27 Oct 2020 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 26 16:22:21 2020

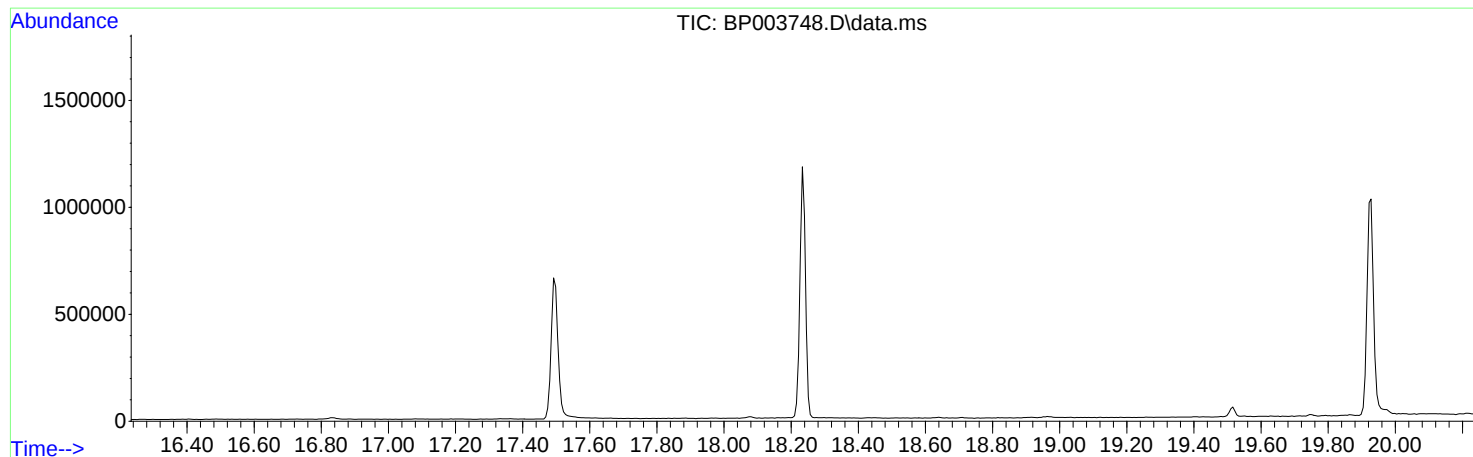

AutoFind: Scans 2608, 2609, 2610; Background Corrected with Scan 2601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	29509	PASS
68	69	0.00	2	1.9	699	PASS
69	198	0.00	100	32.9	36610	PASS
70	69	0.00	2	0.5	186	PASS
127	198	10	80	38.4	42738	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111391	PASS
199	198	5	9	6.7	7490	PASS
275	198	10	60	30.7	34205	PASS
365	198	1	100	3.8	4283	PASS
441	198	0.01	100	15.1	16784	PASS
442	198	50	100	95.8	106704	PASS
443	442	15	24	19.6	20928	PASS