

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012343.D
 Acq On : 27 Oct 2022 14:55
 Operator : CG/JU
 Sample : N5015-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BF0

Quant Time: Oct 27 23:21:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	298730	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	1332662	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.463	164	892568	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.222	188	1961809	20.000	ng/u1	0.00
79) Chrysene-d12	21.316	240	2107934	20.000	ng/u1	0.00
88) Perylene-d12	23.710	264	2102241	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	43474	5.860	ng/uL	0.00
4) Pyridine-d5	3.681	84	106465	4.995	ng/u1	0.00
7) Phenol-d5	6.981	99	863691	32.235	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	517709	32.367	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	671777	34.333	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	710370	33.522	ng/u1	-0.01
21) Nitrobenzene-d5	8.981	128	338974	39.224	ng/u1	0.00
24) 2-Nitrophenol-d4	9.699	143	364647	40.653	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	681520	35.059	ng/u1	0.00
31) 4-Chloroaniline-d4	10.757	131	855996	29.574	ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	2156690	35.297	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	2500868	35.816	ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	288316	24.932	ng/u1	0.00
60) Fluorene-d10	15.457	176	1910346	36.517	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	228969	22.417	ng/u1	0.00
73) Anthracene-d10	17.322	188	3029494	35.839	ng/u1	0.00
81) Pyrene-d10	19.563	212	3640851	34.402	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.557	264	3687953	35.904	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.010	94	38008	1.364	ng/u1	94
16) Acetophenone	8.646	105	42790	1.300	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012343.D
Acq On : 27 Oct 2022 14:55
Operator : CG/JU
Sample : N5015-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BF0

Quant Time: Oct 27 23:21:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration




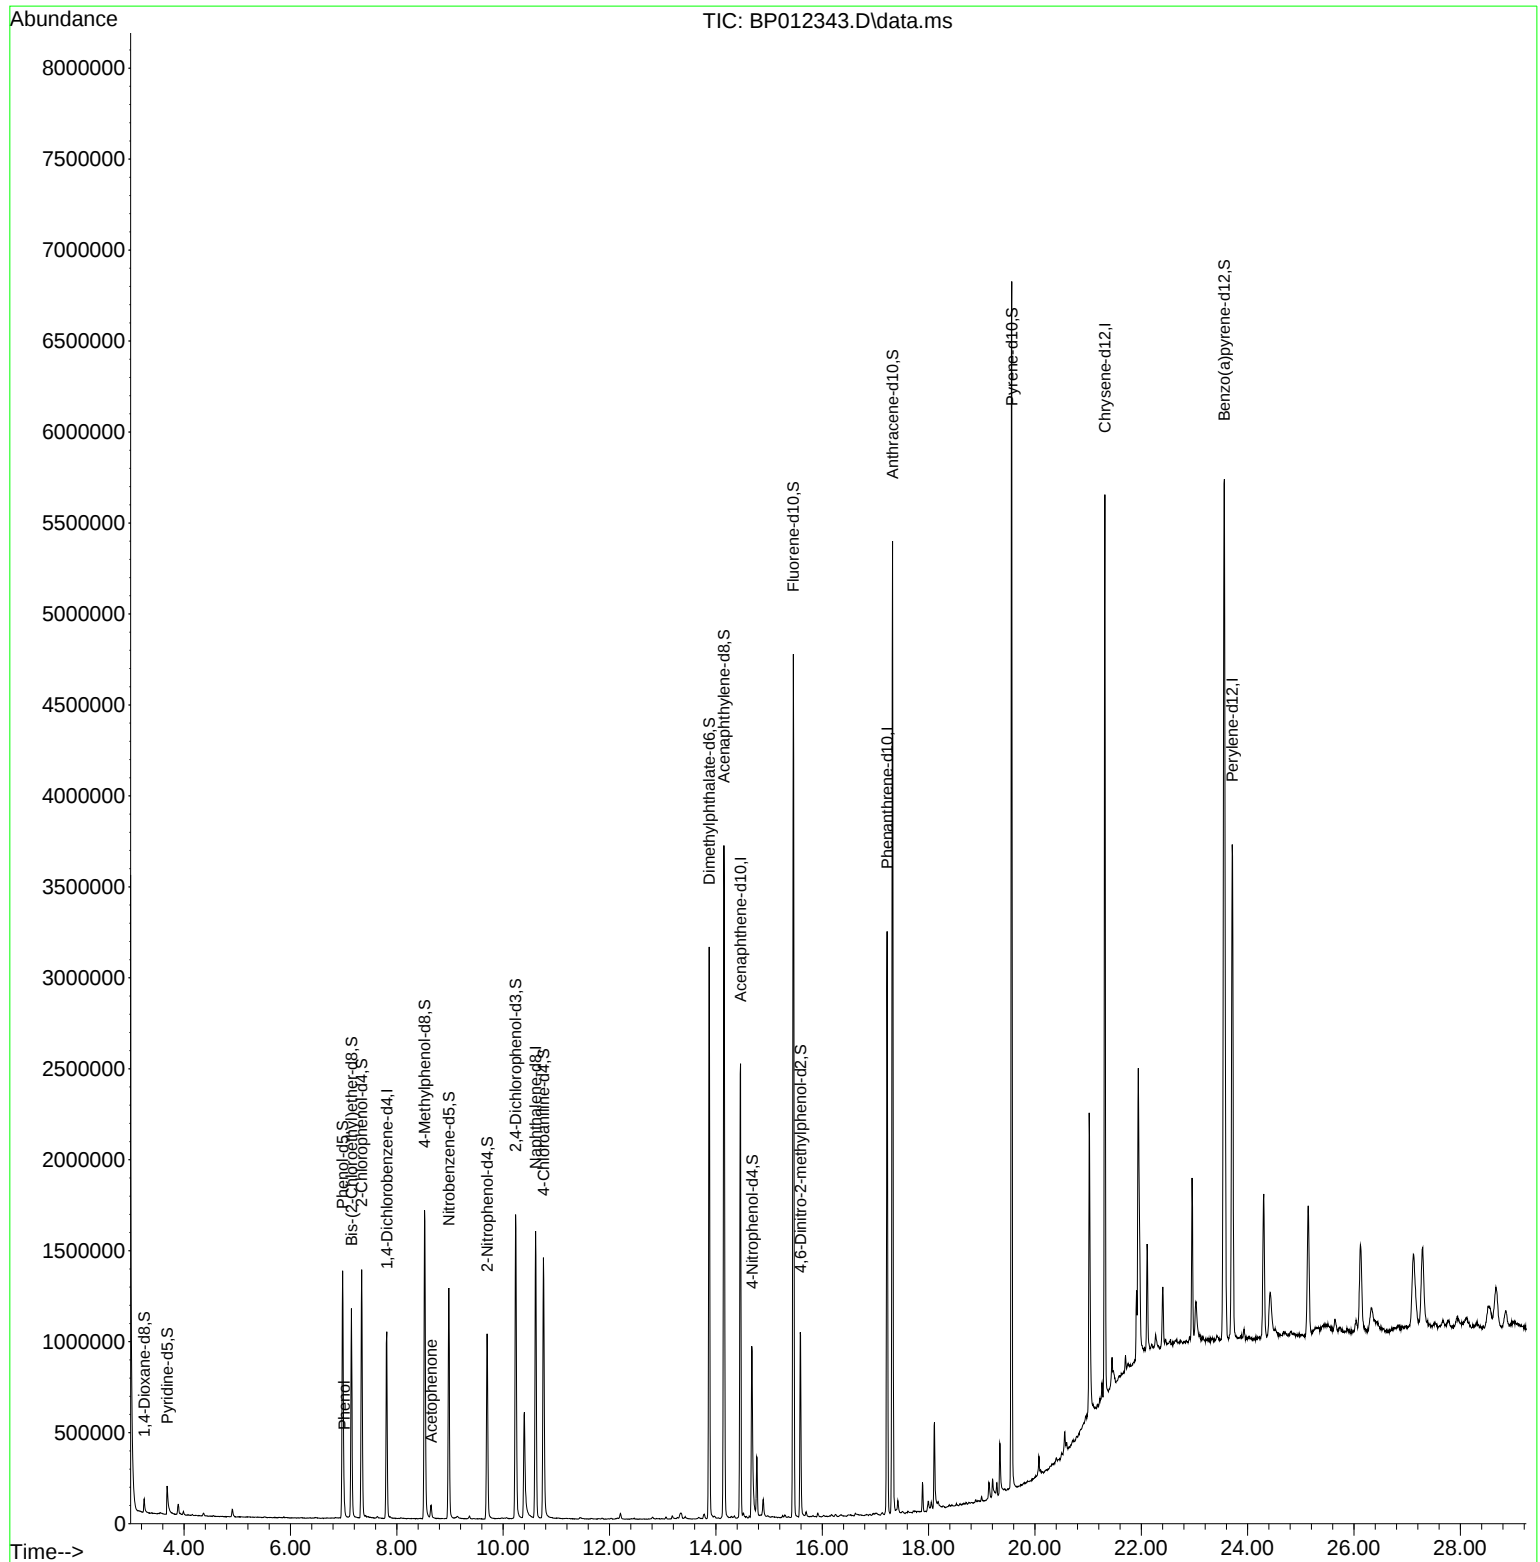


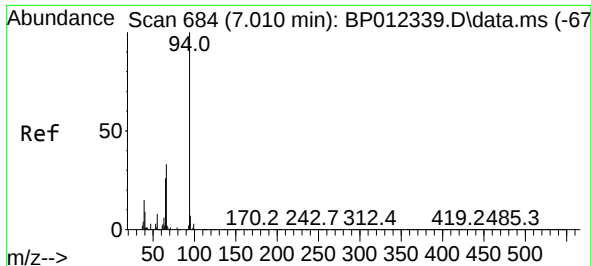

#8
Phenol
Concen: 1.364 ng/ul
RT: 7.010 min Scan# 684
Delta R.T. 0.000 min
Lab File: BP012343.D
Acq: 27 Oct 2022 14:55

Instrument :
BNA_P
ClientSampleId :
C1BF0

Tgt Ion: 94 Resp: 38008
Ion Ratio Lower Upper
94 100
65 26.0 20.8 31.2
66 38.5 26.2 39.2

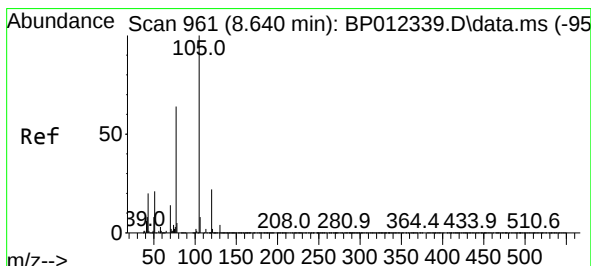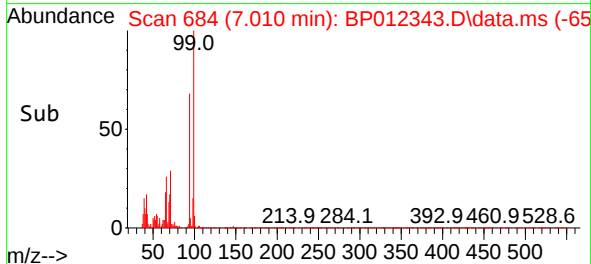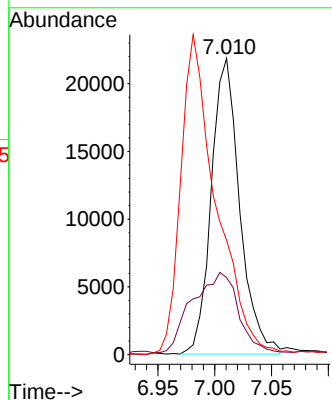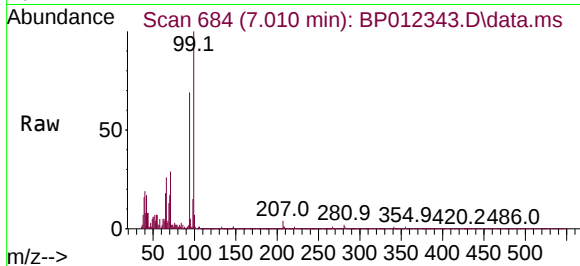

#16
Acetophenone
Concen: 1.300 ng/ul
RT: 8.646 min Scan# 962
Delta R.T. -0.000 min
Lab File: BP012343.D
Acq: 27 Oct 2022 14:55

Tgt Ion: 105 Resp: 42790
Ion Ratio Lower Upper
105 100
77 71.8 60.3 90.5
51 25.9 19.9 29.9

