

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012344.D
 Acq On : 27 Oct 2022 15:29
 Operator : CG/JU
 Sample : N5015-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BE4

Quant Time: Oct 27 23:21:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	301361	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	1350303	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.457	164	897961	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.222	188	1942148	20.000	ng/u1	0.00
79) Chrysene-d12	21.316	240	2065616	20.000	ng/u1	0.00
88) Perylene-d12	23.710	264	2011840	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	34344	4.589	ng/uL	0.00
4) Pyridine-d5	3.693	84	38234	1.778	ng/u1	0.02
7) Phenol-d5	6.981	99	686000	25.379	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	429846	26.639	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	549256	27.826	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	438728	20.522	ng/u1	0.00
21) Nitrobenzene-d5	8.981	128	286454	32.714	ng/u1	0.00
24) 2-Nitrophenol-d4	9.699	143	311857	34.313	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	549288	27.887	ng/u1	0.00
31) 4-Chloroaniline-d4	10.763	131	280736	9.572	ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	1863215	30.311	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	2108158	30.011	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	262700	22.580	ng/u1	0.00
60) Fluorene-d10	15.457	176	1632055	31.010	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	206481	20.420	ng/u1	0.00
73) Anthracene-d10	17.322	188	2392302	28.588	ng/u1	0.00
81) Pyrene-d10	19.563	212	3135752	30.236	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.557	264	3010439	30.625	ng/u1	0.00
Target Compounds						
8) Phenol	7.011	94	36540	1.300	ng/u1#	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012344.D
Acq On : 27 Oct 2022 15:29
Operator : CG/JU
Sample : N5015-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BE4

Quant Time: Oct 27 23:21:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration

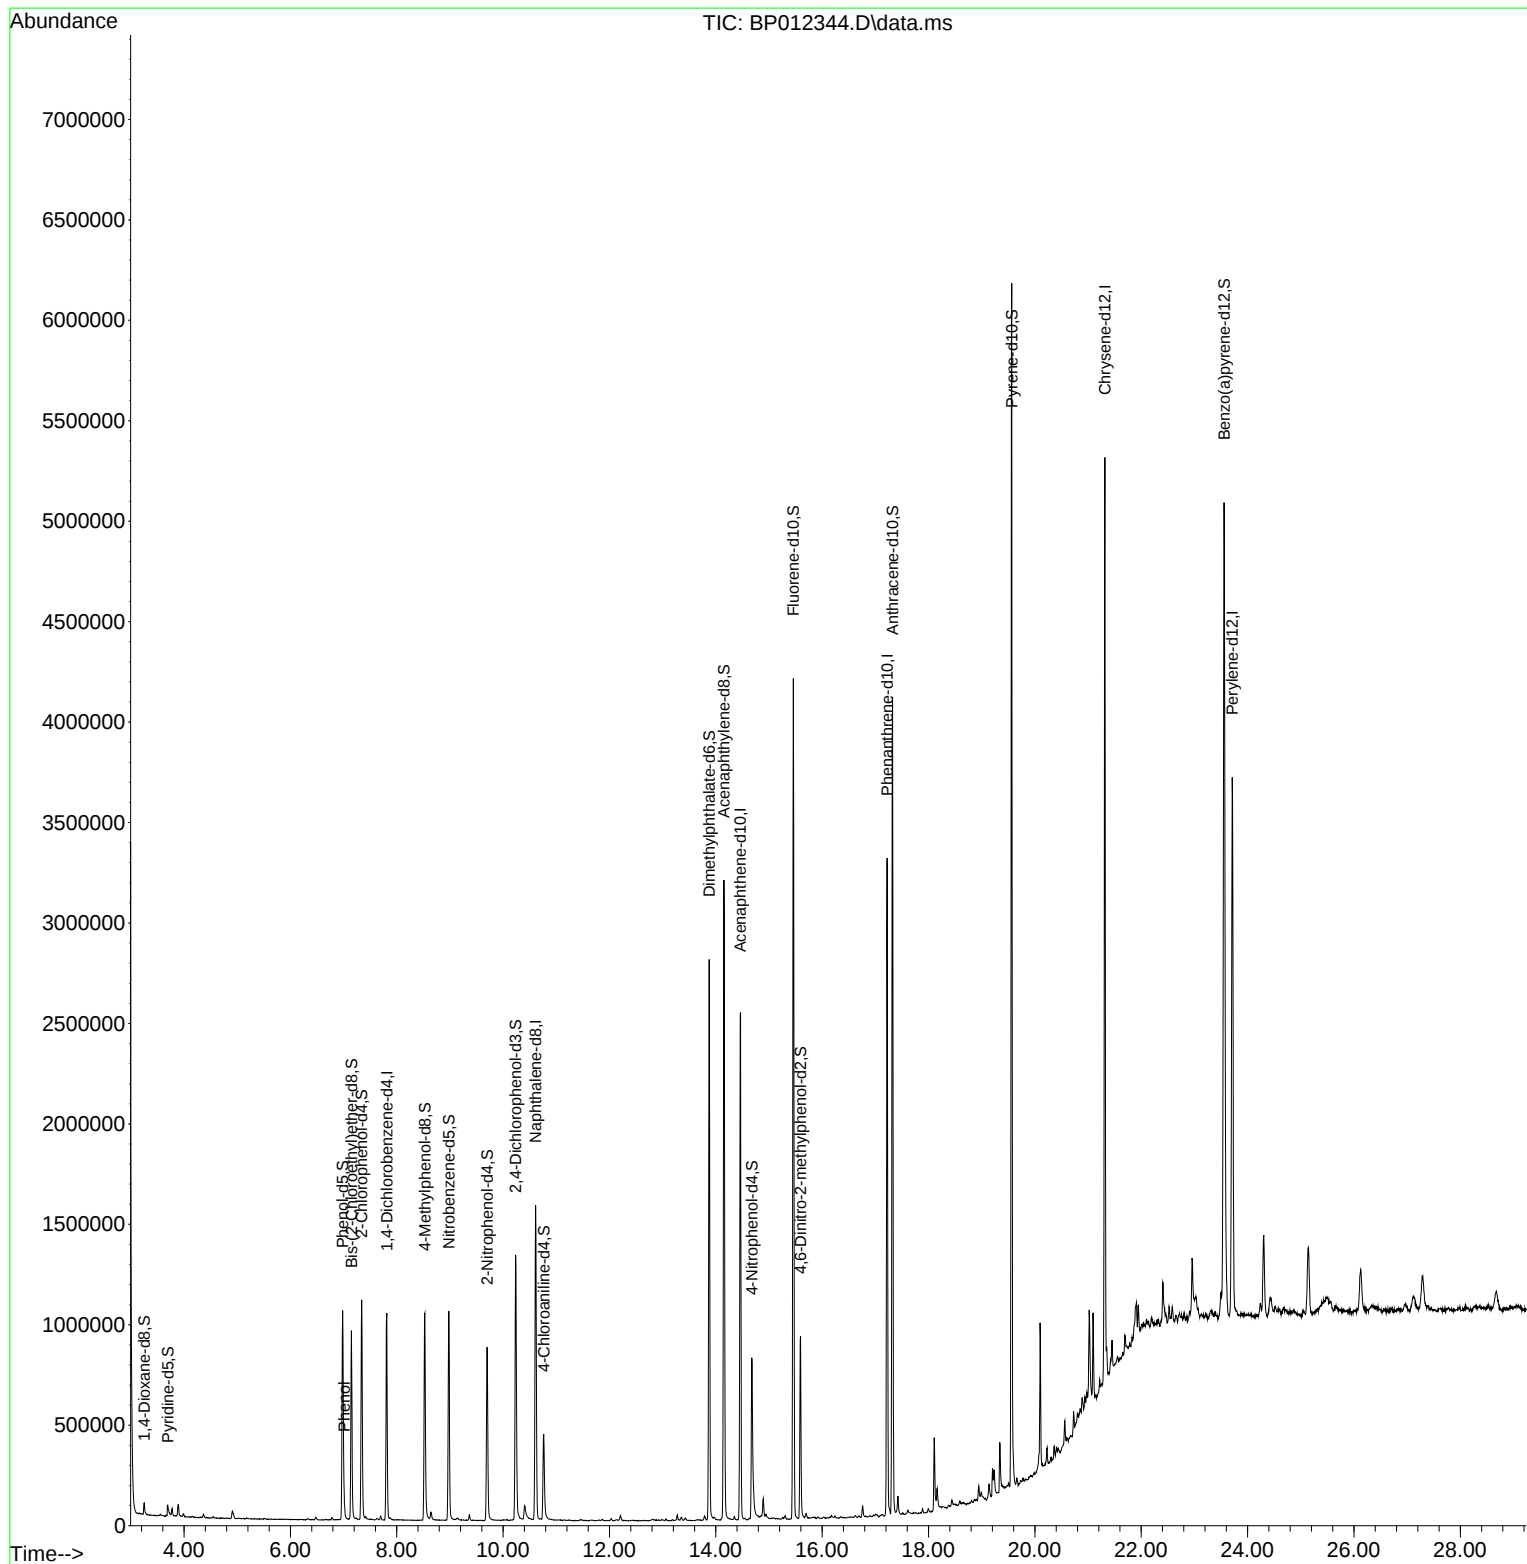

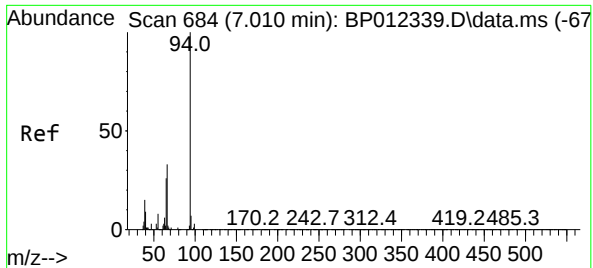

#8
Phenol
Concen: 1.300 ng/ul
RT: 7.011 min Scan# 684
Delta R.T. 0.001 min
Lab File: BP012344.D
Acq: 27 Oct 2022 15:29

Instrument :
BNA_P
ClientSampleId :
C1BE4

Tgt Ion: 94 Resp: 36540
Ion Ratio Lower Upper
94 100
65 25.8 20.8 31.2
66 40.6 26.2 39.2#

