

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012347.D
 Acq On : 27 Oct 2022 17:13
 Operator : CG/JU
 Sample : N5015-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BG0

Quant Time: Oct 27 23:22:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	272798	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	1225458	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.463	164	807442	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.222	188	1780916	20.000	ng/u1	0.00
79) Chrysene-d12	21.316	240	1944107	20.000	ng/u1	0.00
88) Perylene-d12	23.716	264	1879073	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	41761	6.164	ng/uL	0.00
4) Pyridine-d5	3.670	84	567693	29.169	ng/u1	0.00
7) Phenol-d5	6.981	99	877376	35.858	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	530892	36.346	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	679066	38.005	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	710076	36.693	ng/u1	-0.01
21) Nitrobenzene-d5	8.975	128	352582	44.368	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.699	143	392897	47.634	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	687369	38.453	ng/u1	0.00
31) 4-Chloroaniline-d4	10.757	131	1003426	37.700	ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	2182970	39.494	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	2541030	40.228	ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	374732	35.821	ng/u1	0.00
60) Fluorene-d10	15.457	176	1918352	40.536	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	285879	30.832	ng/u1	0.00
73) Anthracene-d10	17.322	188	3038139	39.592	ng/u1	0.00
81) Pyrene-d10	19.563	212	3619118	37.078	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.563	264	3659455	39.857	ng/u1	0.00
Target Compounds						
8) Phenol	7.011	94	36194	1.423	ng/u1#	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012347.D
Acq On : 27 Oct 2022 17:13
Operator : CG/JU
Sample : N5015-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BG0

Quant Time: Oct 27 23:22:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration

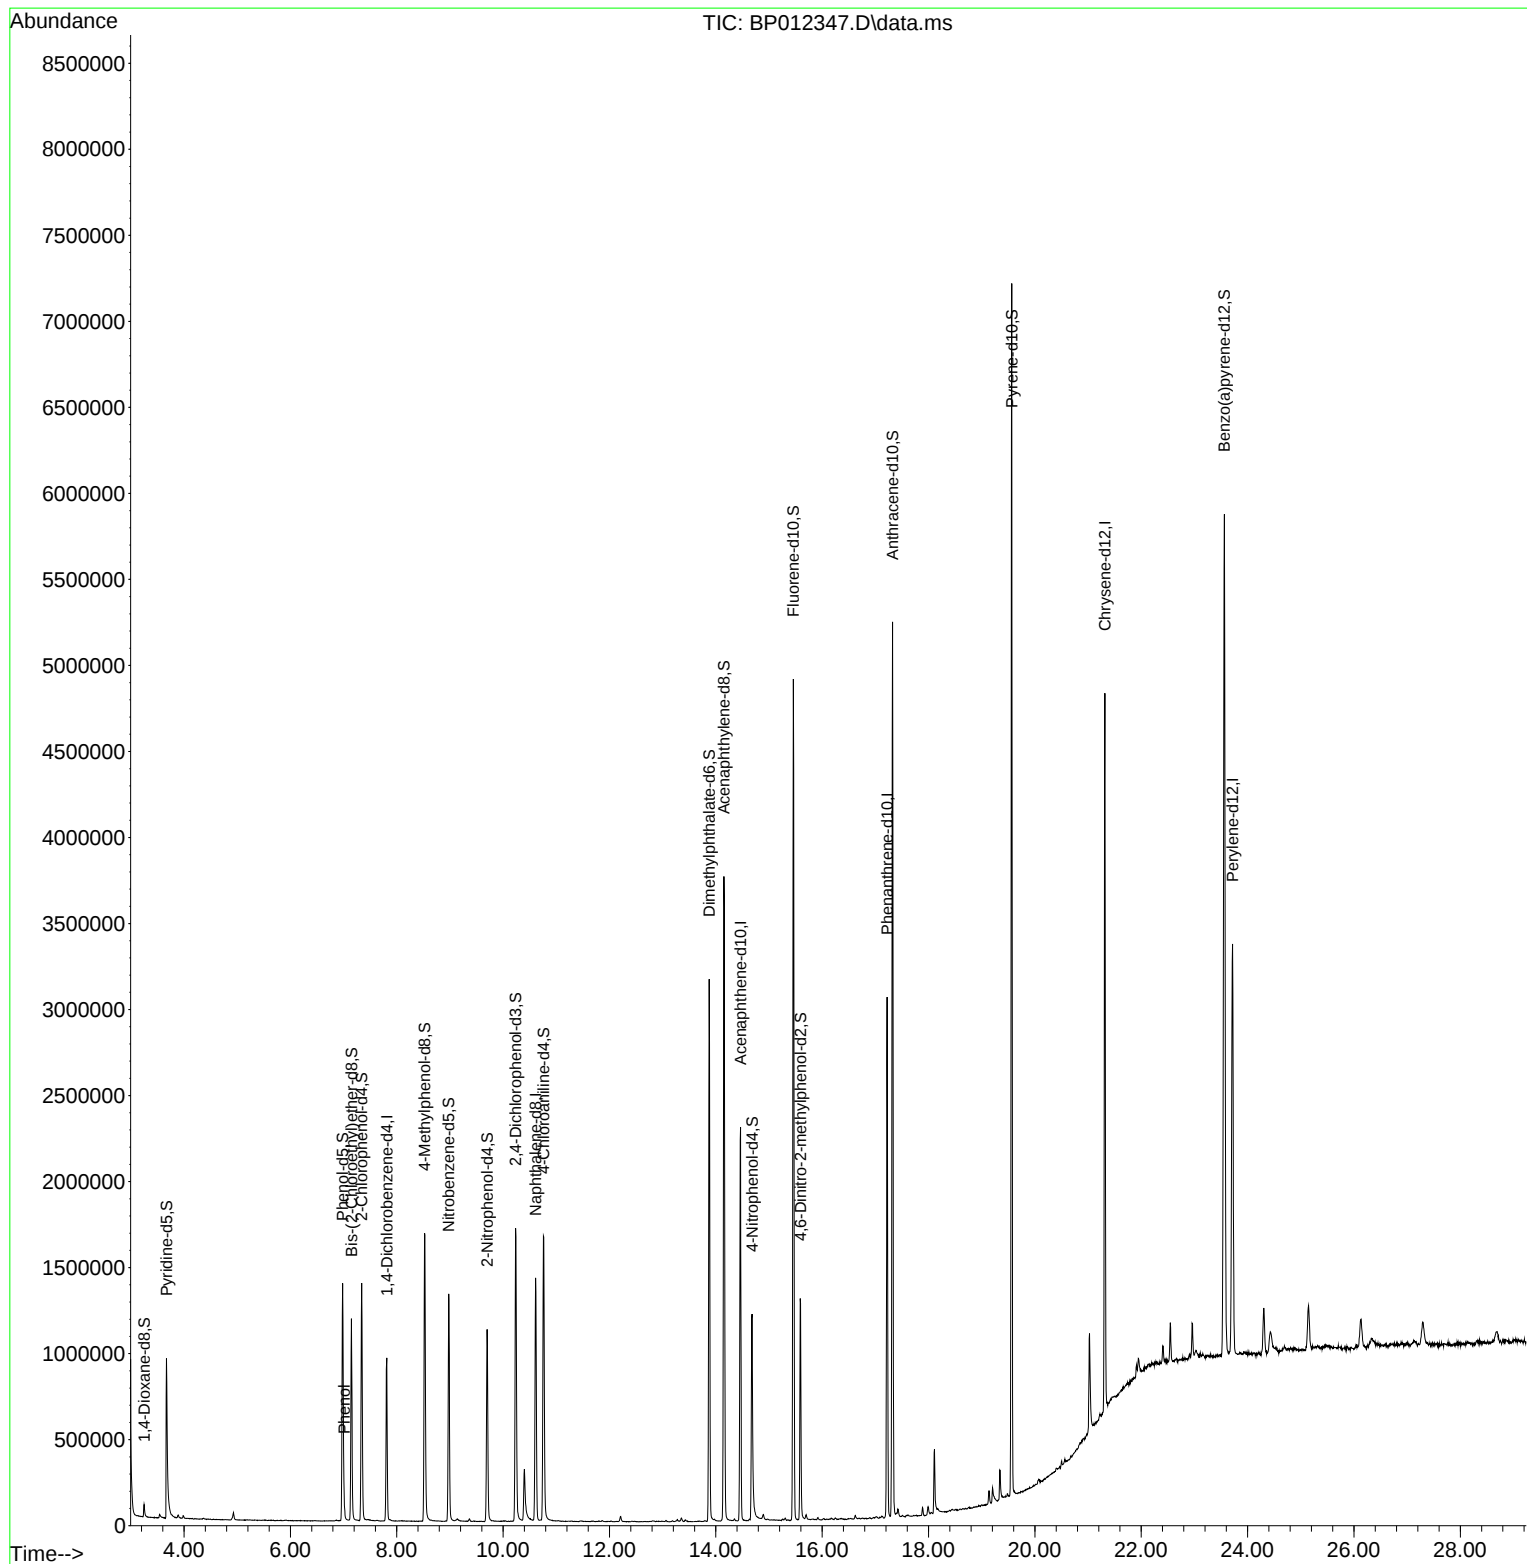

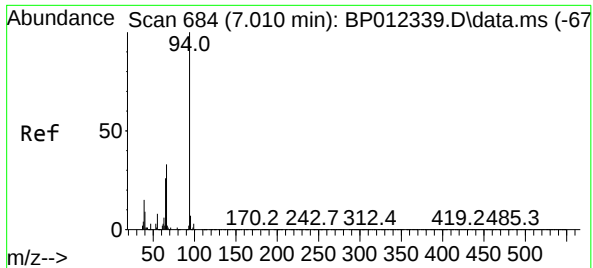

#8
Phenol
Concen: 1.423 ng/ul
RT: 7.011 min Scan# 684
Delta R.T. 0.001 min
Lab File: BP012347.D
Acq: 27 Oct 2022 17:13

Instrument :
BNA_P
ClientSampleId :
C1BG0

Tgt Ion: 94 Resp: 36194
Ion Ratio Lower Upper
94 100
65 29.7 20.8 31.2
66 40.6 26.2 39.2#

