

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012351.D
 Acq On : 27 Oct 2022 20:06
 Operator : CG/JU
 Sample : N5015-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BF9

Quant Time: Oct 27 23:23:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	270603	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.610	136	1165966	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.457	164	752393	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	1686852	20.000	ng/u1	0.00
79) Chrysene-d12	21.316	240	1945500	20.000	ng/u1	0.00
88) Perylene-d12	23.710	264	1999594	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	44711	6.653	ng/uL	0.00
4) Pyridine-d5	3.681	84	105050	5.441	ng/u1	0.00
7) Phenol-d5	6.981	99	852661	35.131	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	515493	35.578	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	664235	37.476	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	589737	30.722	ng/u1	-0.01
21) Nitrobenzene-d5	8.975	128	333853	44.154	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.699	143	365123	46.525	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	623732	36.674	ng/u1	0.00
31) 4-Chloroaniline-d4	10.758	131	839013	33.131	ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	2108377	40.935	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	2357008	40.045	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	330953	33.951	ng/u1	0.00
60) Fluorene-d10	15.457	176	1826495	41.419	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.587	200	254318	28.957	ng/u1	0.00
73) Anthracene-d10	17.316	188	2896556	39.852	ng/u1	0.00
81) Pyrene-d10	19.557	212	3753406	38.427	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.557	264	3989423	40.832	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.005	94	36707	1.455	ng/u1#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012351.D
Acq On : 27 Oct 2022 20:06
Operator : CG/JU
Sample : N5015-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BF9

Quant Time: Oct 27 23:23:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration

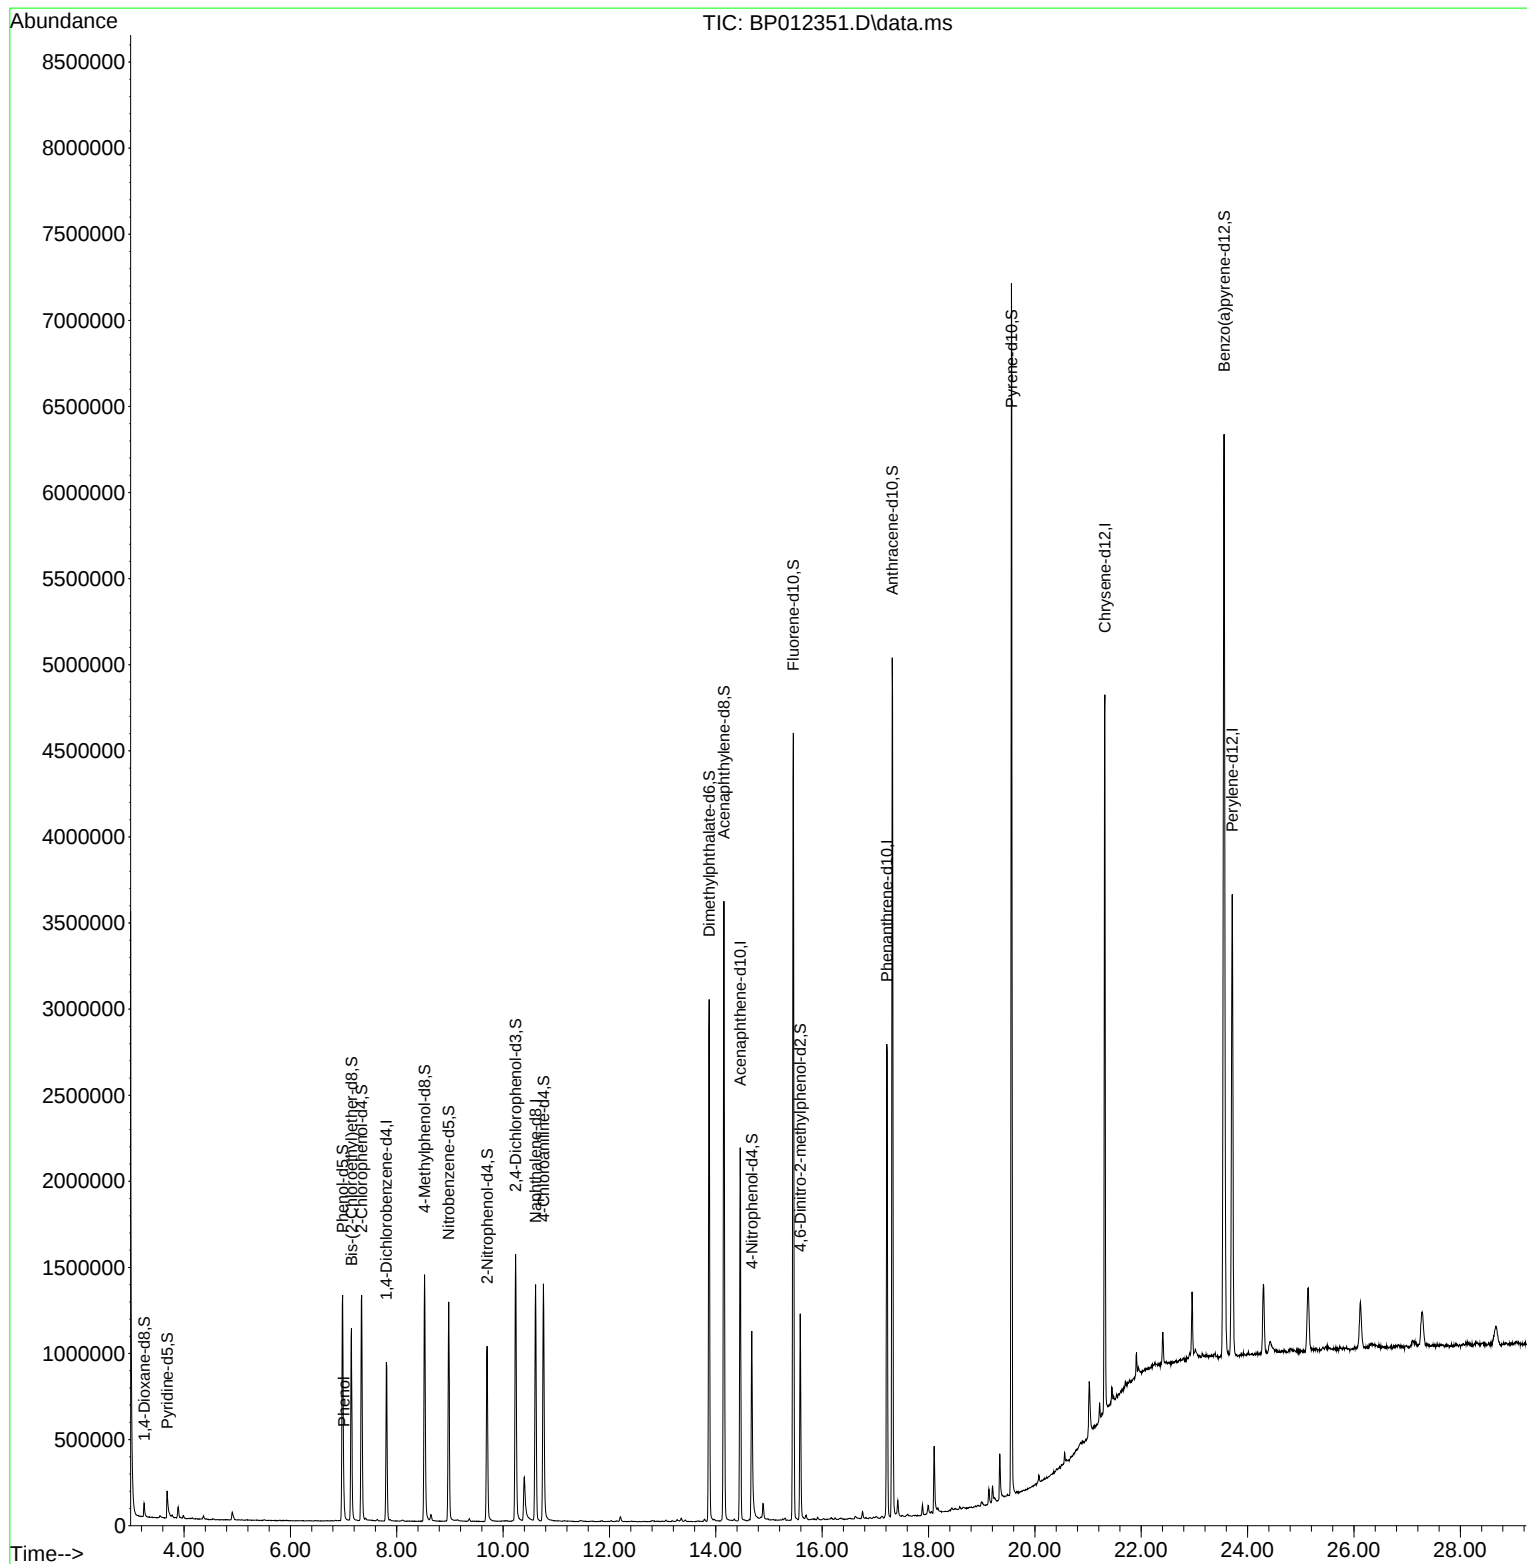

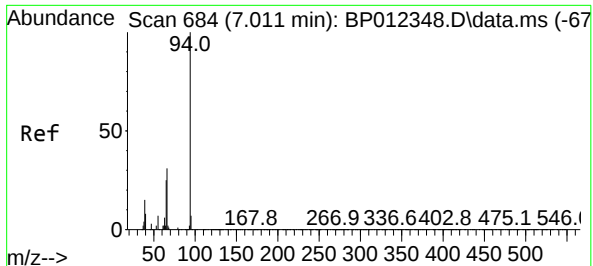

#8
Phenol
Concen: 1.455 ng/ul
RT: 7.005 min Scan# 68
Delta R.T. -0.005 min
Lab File: BP012351.D
Acq: 27 Oct 2022 20:06

Instrument :
BNA_P
ClientSampleId :
C1BF9

Tgt Ion: 94 Resp: 36707
Ion Ratio Lower Upper
94 100
65 28.4 20.8 31.2
66 40.0 26.2 39.2#

