

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012352.D
 Acq On : 27 Oct 2022 20:40
 Operator : CG/JU
 Sample : N5015-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BE8

Quant Time: Oct 27 23:23:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	319952	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.610	136	1448510	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.457	164	982051	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	2190713	20.000	ng/u1	0.00
79) Chrysene-d12	21.316	240	2201428	20.000	ng/u1	0.00
88) Perylene-d12	23.710	264	1989614	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	45533	5.730	ng/uL	0.00
4) Pyridine-d5	3.681	84	122332	5.359	ng/u1	0.00
7) Phenol-d5	6.981	99	884703	30.829	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	550667	32.144	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	694018	33.117	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	692376	30.505	ng/u1	-0.01
21) Nitrobenzene-d5	8.975	128	356416	37.944	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.699	143	395417	40.557	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	705861	33.407	ng/u1	0.00
31) 4-Chloroaniline-d4	10.757	131	936214	29.758	ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	2442310	36.329	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	2699610	35.139	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	390208	30.669	ng/u1	0.00
60) Fluorene-d10	15.457	176	2135881	37.108	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.587	200	311236	27.288	ng/u1	0.00
73) Anthracene-d10	17.316	188	3409875	36.124	ng/u1	0.00
81) Pyrene-d10	19.557	212	4094101	37.042	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.557	264	3666291	37.713	ng/u1	0.00
Target Compounds						Qvalue
8) Phenol	7.005	94	38115	1.277	ng/u1#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012352.D
Acq On : 27 Oct 2022 20:40
Operator : CG/JU
Sample : N5015-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BE8

Quant Time: Oct 27 23:23:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration

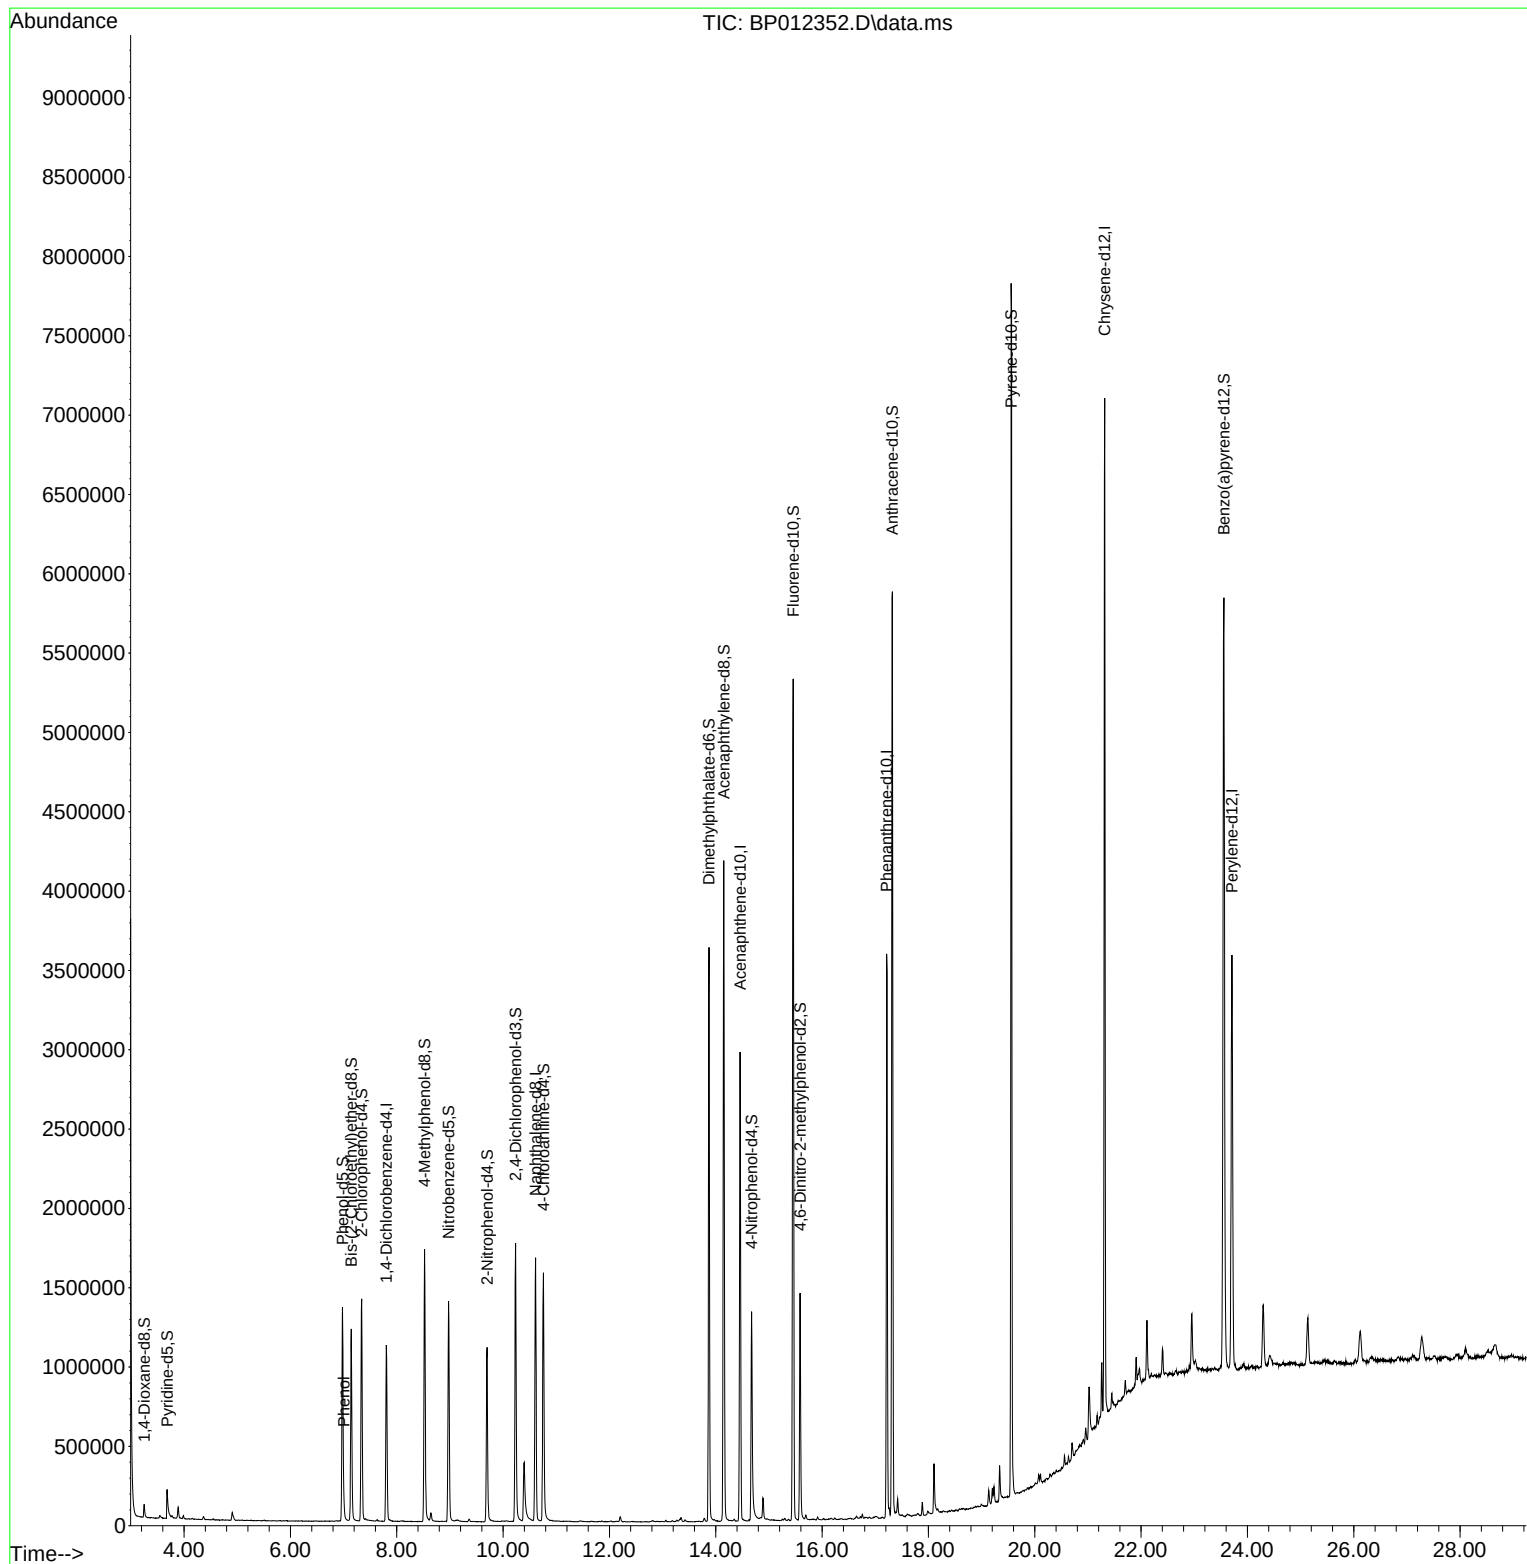

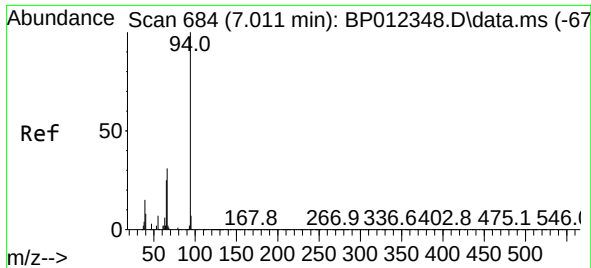

#8
Phenol
Concen: 1.277 ng/ul
RT: 7.005 min Scan# 68
Delta R.T. -0.005 min
Lab File: BP012352.D
Acq: 27 Oct 2022 20:40

Instrument :
BNA_P
ClientSampleId :
C1BE8

Tgt Ion: 94 Resp: 38115
Ion Ratio Lower Upper
94 100
65 26.9 20.8 31.2
66 44.2 26.2 39.2#

