

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012353.D
 Acq On : 27 Oct 2022 21:15
 Operator : CG/JU
 Sample : N5015-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BG1

Quant Time: Oct 27 23:23:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	330775	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.610	136	1492157	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.457	164	1005390	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.222	188	2195930	20.000	ng/u1	0.00
79) Chrysene-d12	21.315	240	2185226	20.000	ng/u1	0.00
88) Perylene-d12	23.709	264	1914417	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	63549	7.736	ng/uL	0.00
4) Pyridine-d5	3.675	84	289936	12.286	ng/u1	0.00
7) Phenol-d5	6.981	99	1317412	44.405	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	803550	45.371	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	1024561	47.290	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	1004293	42.800	ng/u1	-0.01
21) Nitrobenzene-d5	8.975	128	541369	55.948	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.698	143	598116	59.553	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	1049039	48.197	ng/u1	0.00
31) 4-Chloroaniline-d4	10.757	131	1414019	43.631	ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	3342181	48.561	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	3784407	48.116	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	557466	42.797	ng/u1	0.00
60) Fluorene-d10	15.457	176	2890597	49.055	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.586	200	431352	37.729	ng/u1	0.00
73) Anthracene-d10	17.322	188	4465443	47.195	ng/u1	0.00
81) Pyrene-d10	19.563	212	5321521	48.504	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.557	264	4696029	50.203	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.004	94	54451	1.765	ng/u1#	86
16) Acetophenone	8.640	105	37976	1.042	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012353.D
Acq On : 27 Oct 2022 21:15
Operator : CG/JU
Sample : N5015-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BG1

Quant Time: Oct 27 23:23:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration




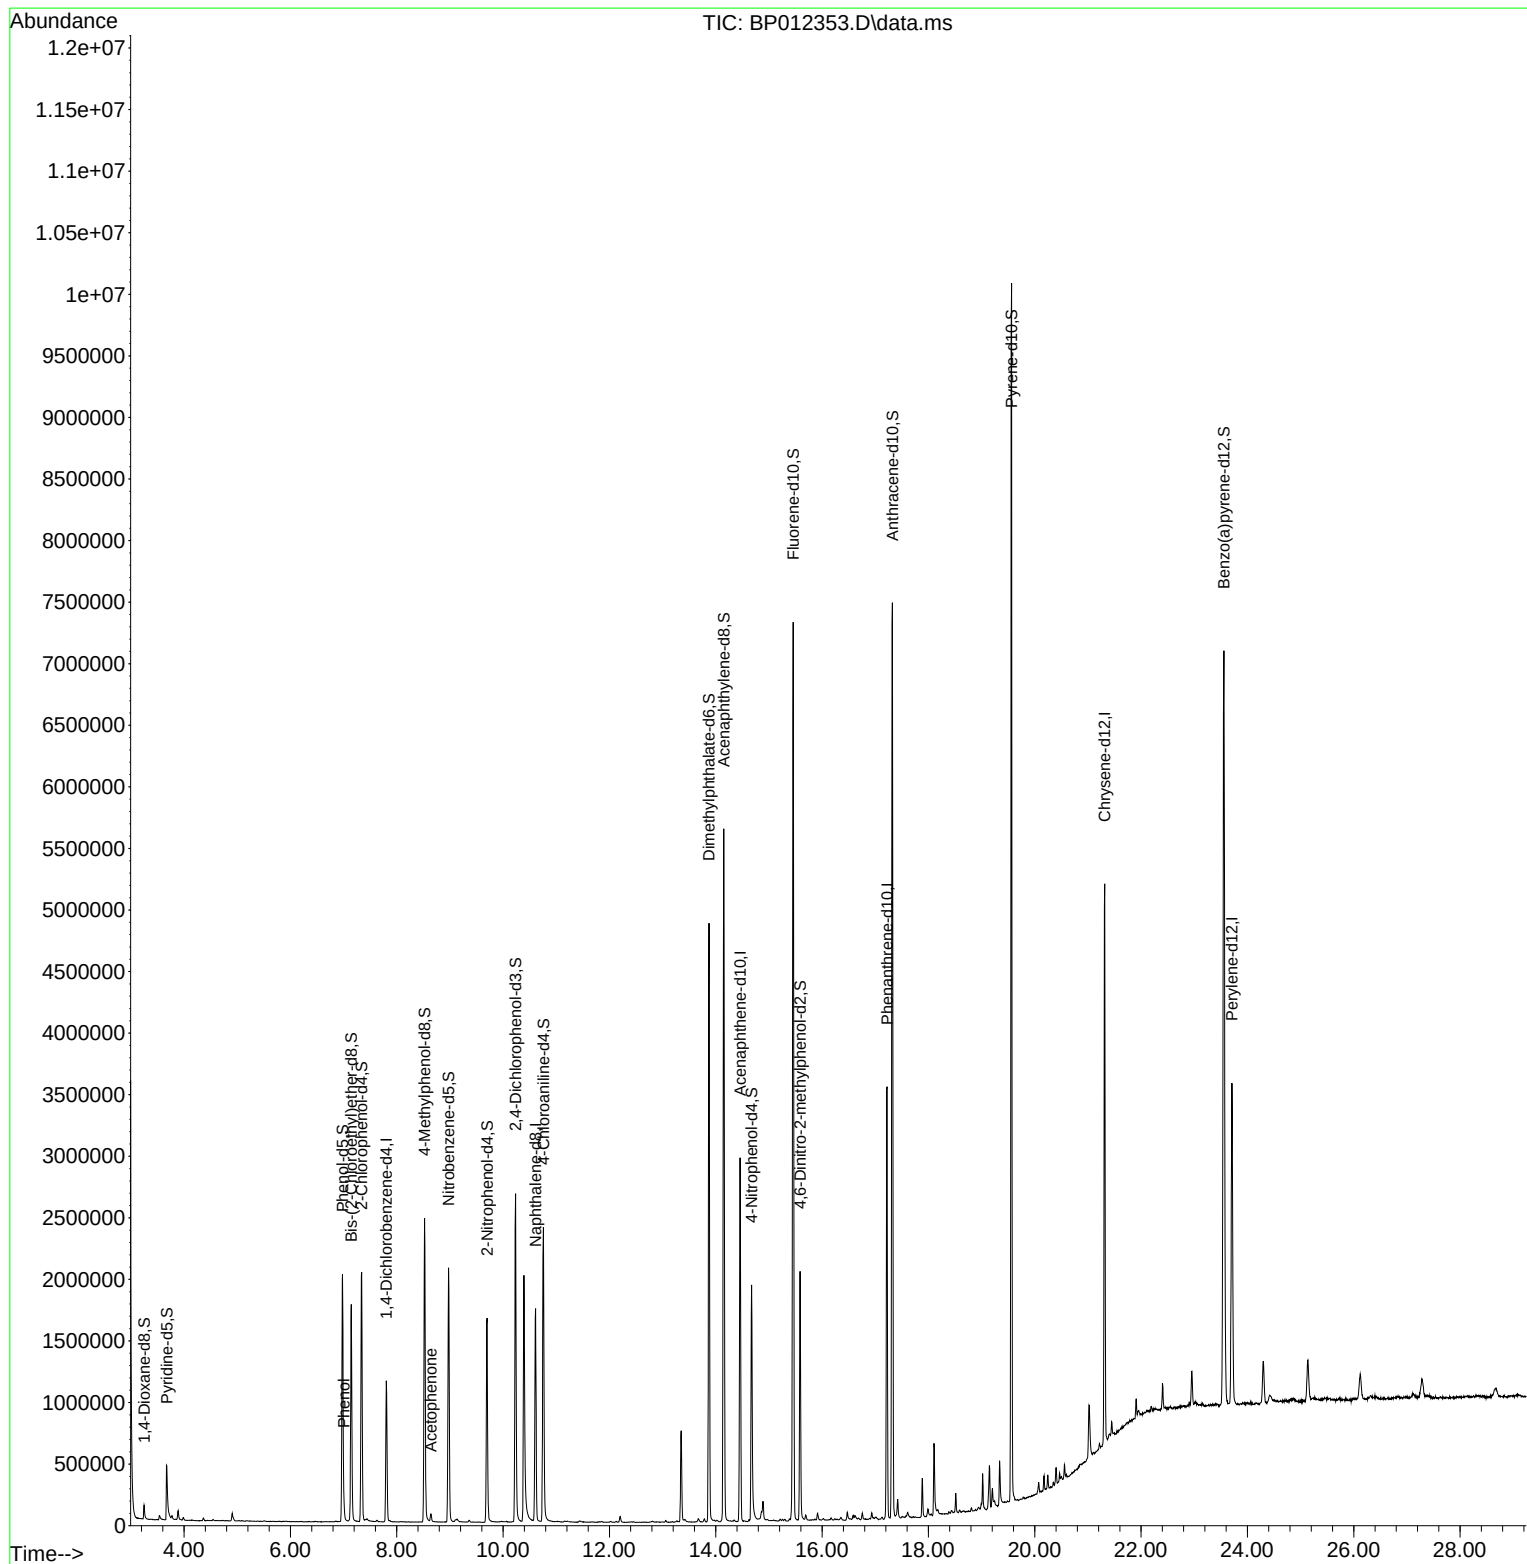


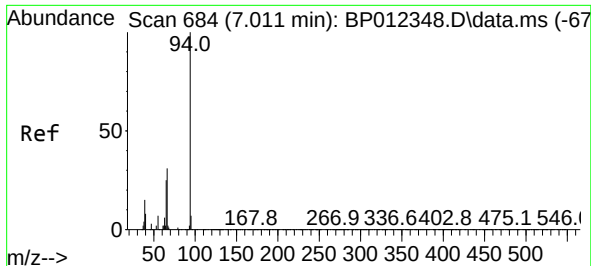

#8
Phenol
Concen: 1.765 ng/ul
RT: 7.004 min Scan# 684
Delta R.T. -0.006 min
Lab File: BP012353.D
Acq: 27 Oct 2022 21:15

Instrument :
BNA_P
ClientSampleId :
C1BG1

Tgt Ion: 94 Resp: 54451
Ion Ratio Lower Upper
94 100
65 30.2 20.8 31.2
66 42.8 26.2 39.2#

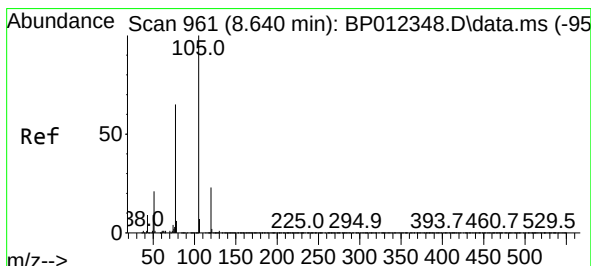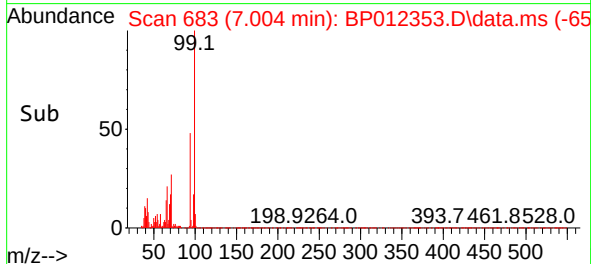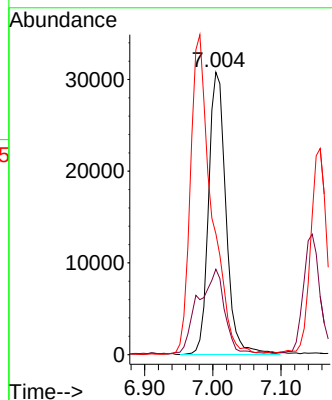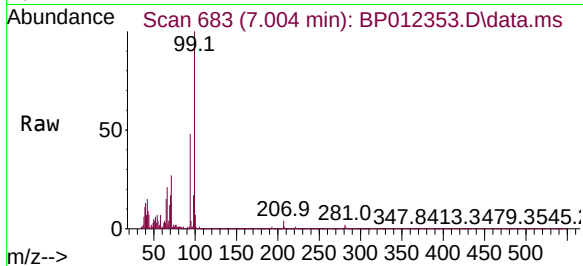

#16
Acetophenone
Concen: 1.042 ng/ul
RT: 8.640 min Scan# 961
Delta R.T. -0.006 min
Lab File: BP012353.D
Acq: 27 Oct 2022 21:15

Tgt Ion: 105 Resp: 37976
Ion Ratio Lower Upper
105 100
77 72.5 60.3 90.5
51 23.8 19.9 29.9

