

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012354.D
 Acq On : 27 Oct 2022 21:49
 Operator : CG/JU
 Sample : N5015-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C1BG2

Quant Time: Oct 27 23:24:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.805	152	328730	20.000 ng/u1	-0.01
20) Naphthalene-d8	10.610	136	1456248	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.457	164	960776	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.216	188	2103975	20.000 ng/u1	0.00
79) Chrysene-d12	21.310	240	2185568	20.000 ng/u1	0.00
88) Perylene-d12	23.710	264	2018345	20.000 ng/u1	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.246	96	54099	6.626 ng/uL	0.00
4) Pyridine-d5	3.676	84	160441	6.841 ng/u1	0.00
7) Phenol-d5	6.981	99	1078704	36.585 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	670048	38.068 ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	857161	39.810 ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	778754	33.395 ng/u1	-0.01
21) Nitrobenzene-d5	8.975	128	447860	47.425 ng/u1	-0.01
24) 2-Nitrophenol-d4	9.699	143	491578	50.152 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	874616	41.174 ng/u1	0.00
31) 4-Chloroaniline-d4	10.757	131	1115985	35.284 ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	2779827	42.266 ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	3187578	42.410 ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	454693	36.528 ng/u1	0.00
60) Fluorene-d10	15.457	176	2439088	43.315 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.587	200	323792	29.559 ng/u1	0.00
73) Anthracene-d10	17.316	188	3630930	40.052 ng/u1	0.00
81) Pyrene-d10	19.557	212	4598867	41.911 ng/u1	0.00
92) Benzo(a)pyrene-d12	23.557	264	4276745	43.366 ng/u1	0.00
Target Compounds					
8) Phenol	7.005	94	39667	1.294 ng/u1#	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012354.D
Acq On : 27 Oct 2022 21:49
Operator : CG/JU
Sample : N5015-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C1BG2

Quant Time: Oct 27 23:24:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration

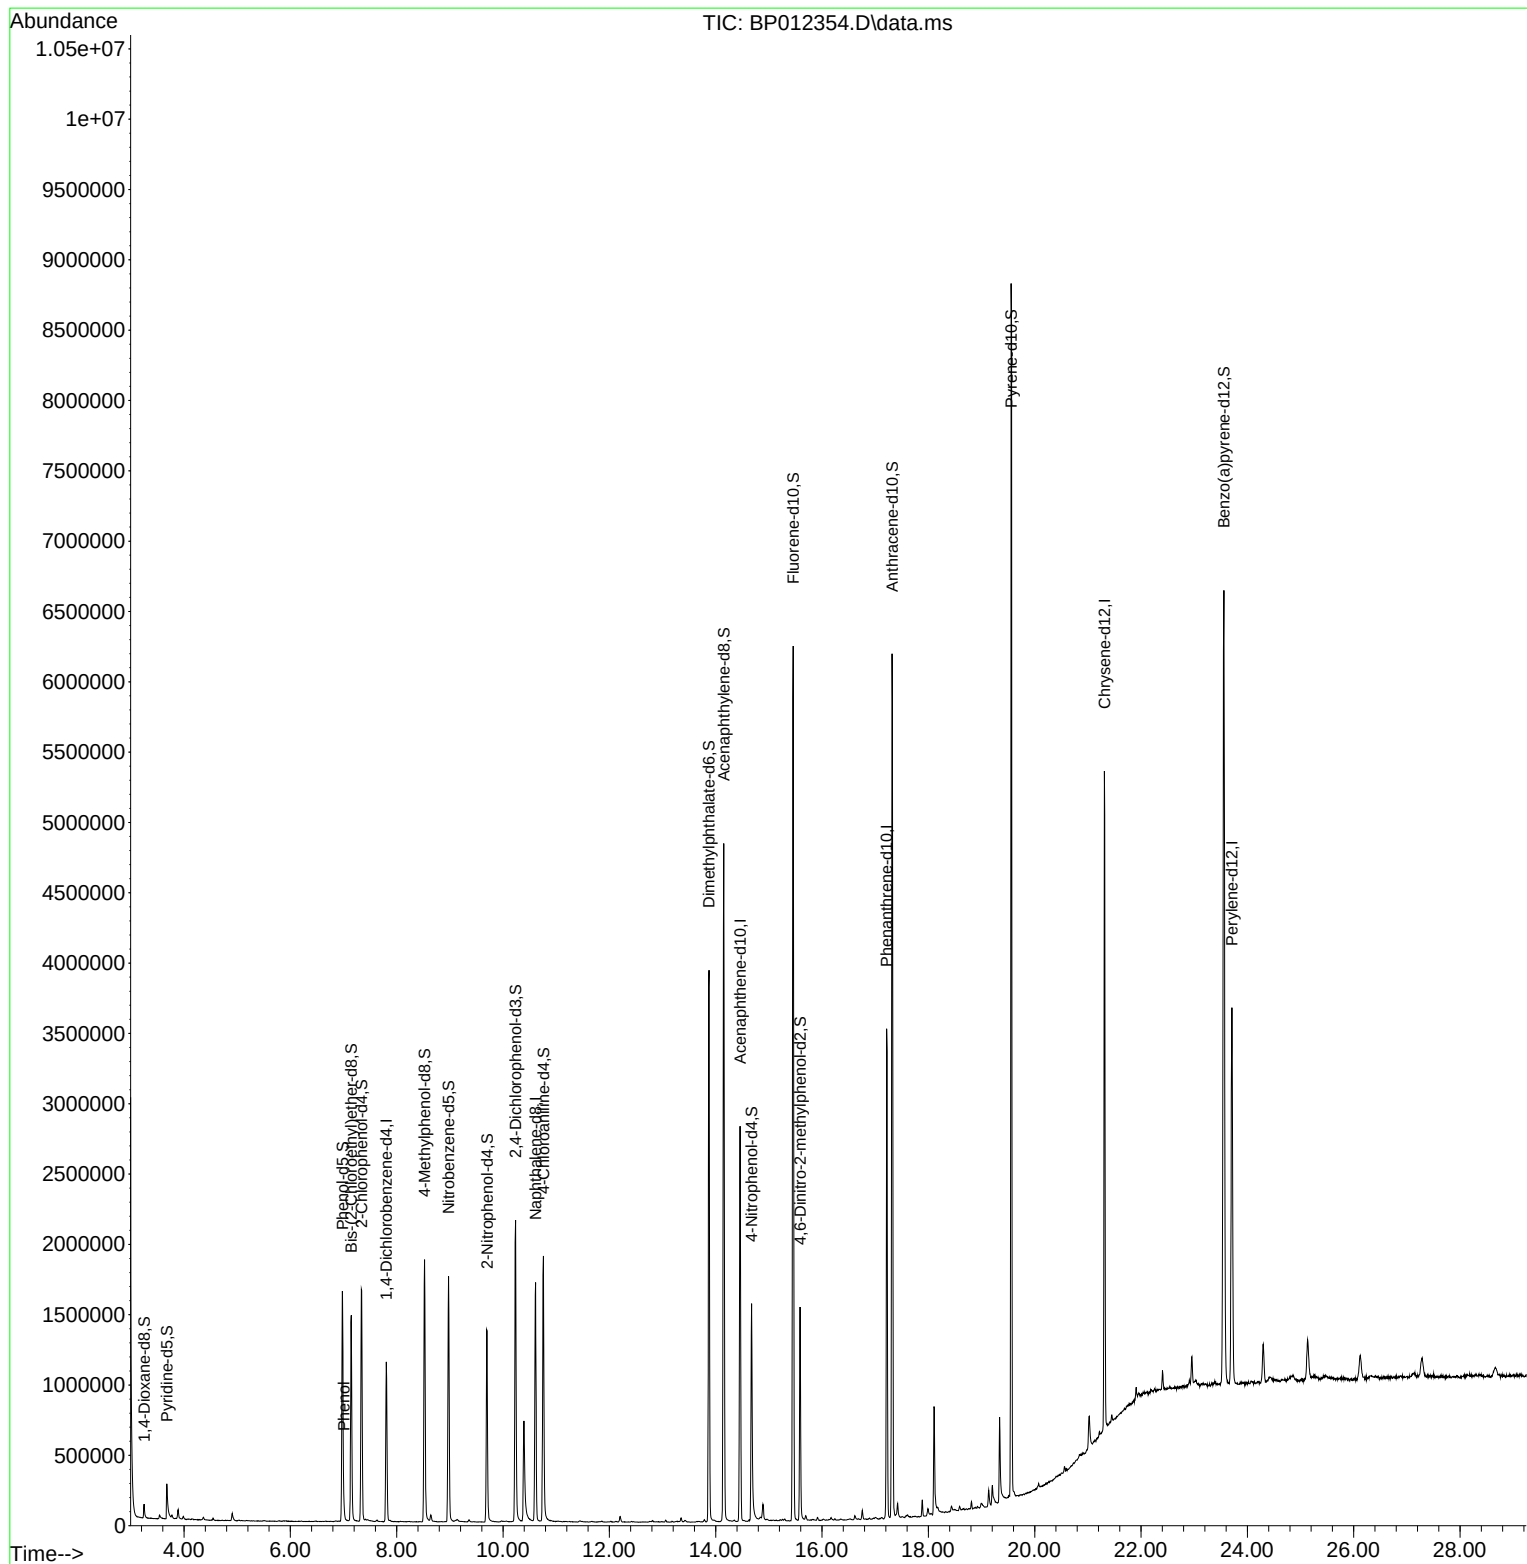

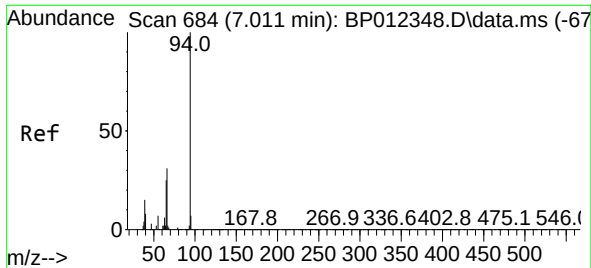

#8
Phenol
Concen: 1.294 ng/ul
RT: 7.005 min Scan# 68
Delta R.T. -0.005 min
Lab File: BP012354.D
Acq: 27 Oct 2022 21:49

Instrument :
BNA_P
ClientSampleId :
C1BG2

Tgt Ion: 94 Resp: 39667
Ion Ratio Lower Upper
94 100
65 27.2 20.8 31.2
66 40.9 26.2 39.2#

