

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012362.D
 Acq On : 28 Oct 2022 02:21
 Operator : CG/JU
 Sample : N5144-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BR1

Quant Time: Oct 28 04:17:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 26 23:40:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	248554	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.605	136	1146358	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.457	164	770916	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	1693735	20.000	ng/u1	0.00
79) Chrysene-d12	21.310	240	1836804	20.000	ng/u1	0.00
88) Perylene-d12	23.704	264	1823217	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	22028	3.568	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.975	99	433711	19.455	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.140	67	281658	21.164	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.334	132	345027	21.193	ng/u1	-0.01
15) 4-Methylphenol-d8	8.522	113	301676	17.110	ng/u1	-0.01
21) Nitrobenzene-d5	8.975	128	184989	24.885	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.693	143	194522	25.211	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.234	165	352766	21.096	ng/u1	0.00
31) 4-Chloroaniline-d4	10.758	131	384337	15.437	ng/u1	0.00
46) Dimethylphthalate-d6	13.869	166	1210864	22.945	ng/u1	-0.01
49) Acenaphthylene-d8	14.146	160	1380350	22.888	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.675	143	162262	16.246	ng/u1	0.00
60) Fluorene-d10	15.451	176	1132371	25.062	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.587	200	116062	13.161	ng/u1	0.00
73) Anthracene-d10	17.316	188	1811277	24.819	ng/u1	0.00
81) Pyrene-d10	19.557	212	2216631	24.036	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.551	264	2148289	24.115	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.005	94	43718	1.886	ng/u1	96
16) Acetophenone	8.640	105	121996	4.455	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012362.D
Acq On : 28 Oct 2022 02:21
Operator : CG/JU
Sample : N5144-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BR1

Quant Time: Oct 28 04:17:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 26 23:40:20 2022
Response via : Initial Calibration




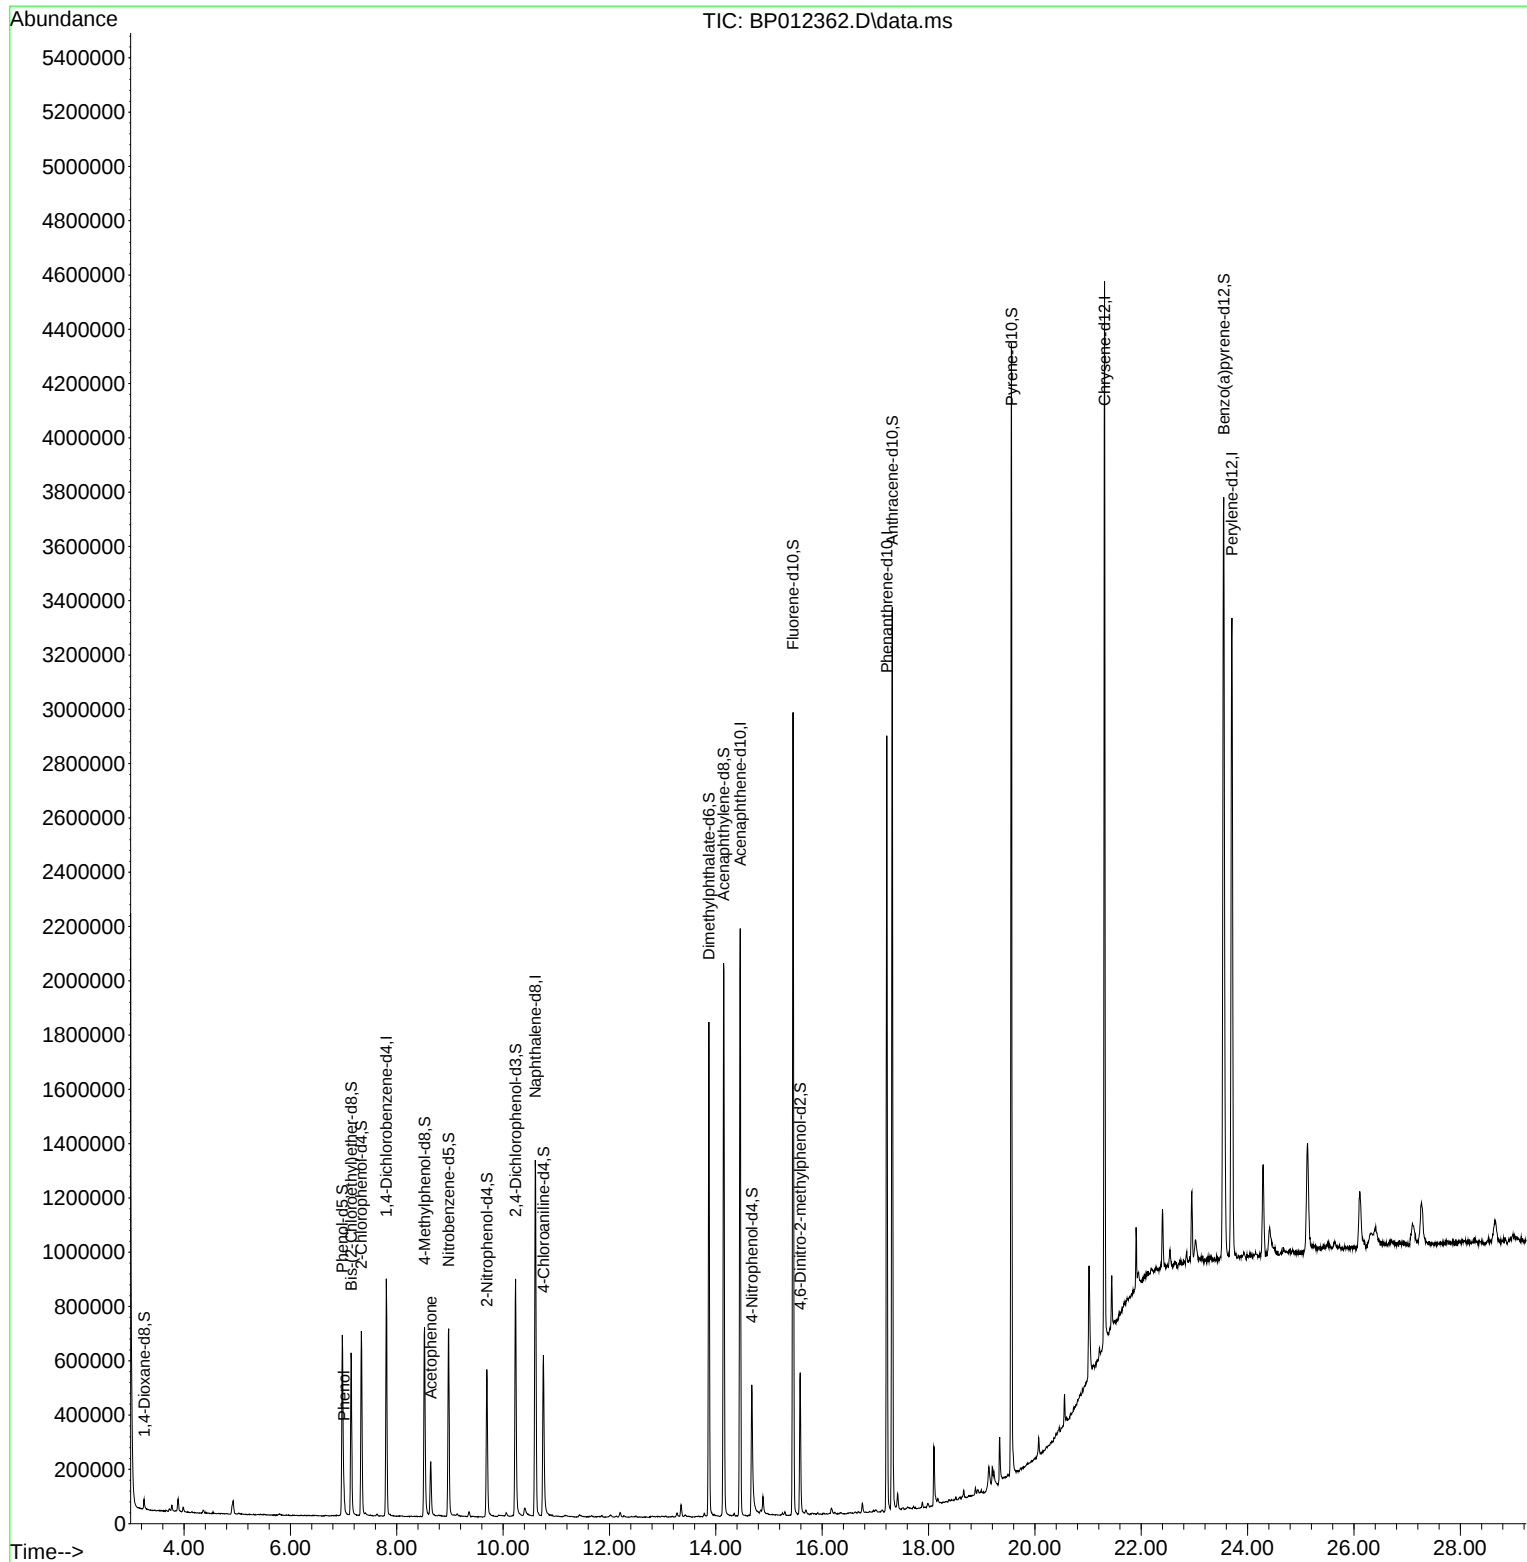


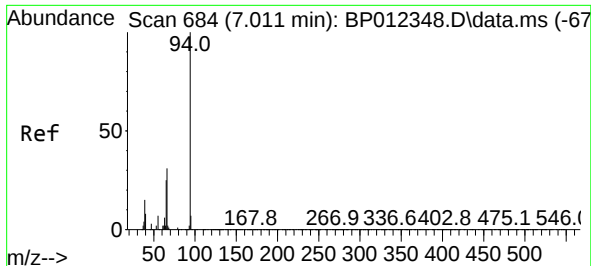

#8
Phenol
Concen: 1.886 ng/ul
RT: 7.005 min Scan# 684
Delta R.T. -0.005 min
Lab File: BP012362.D
Acq: 28 Oct 2022 02:21

Instrument :
BNA_P
ClientSampleId :
C0BR1

Tgt Ion: 94 Resp: 43718
Ion Ratio Lower Upper
94 100
65 26.2 20.8 31.2
66 37.0 26.2 39.2

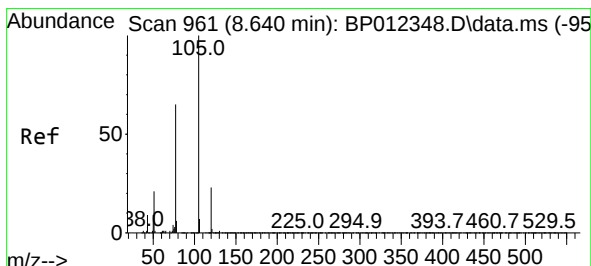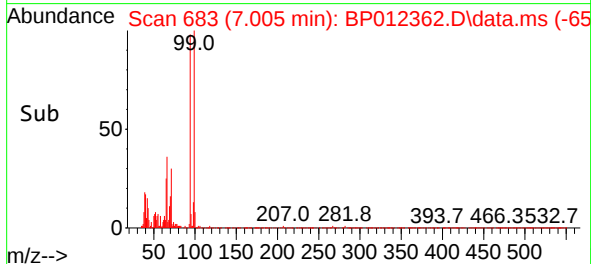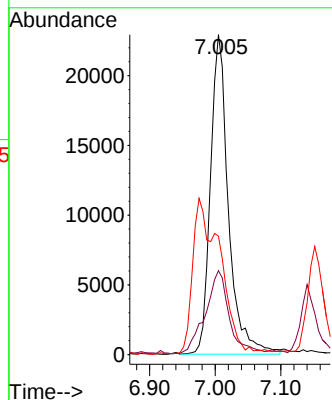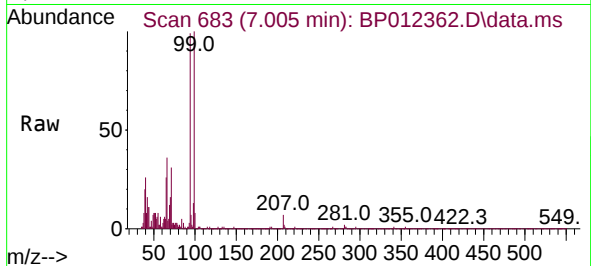

#16
Acetophenone
Concen: 4.455 ng/ul
RT: 8.640 min Scan# 961
Delta R.T. -0.006 min
Lab File: BP012362.D
Acq: 28 Oct 2022 02:21

Tgt Ion: 105 Resp: 121996
Ion Ratio Lower Upper
105 100
77 75.6 60.3 90.5
51 23.4 19.9 29.9

