

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012340.D
 Acq On : 27 Oct 2022 12:36
 Operator : CG/JU
 Sample : PB148454BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK454

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	41	44	55	rVB	50461	79663	1.04%	0.119%
2	3.681	115	118	146	rBV	196464	407561	5.30%	0.611%
3	3.987	166	170	175	rVB	12125	16578	0.22%	0.025%
4	6.981	673	679	692	rBV	856014	1439691	18.71%	2.158%
5	7.146	700	707	723	rBV	746208	1216033	15.81%	1.823%
6	7.340	732	740	757	rBV	866110	1466526	19.06%	2.198%
7	7.811	813	820	832	rBV	738440	1200338	15.60%	1.799%
8	8.528	934	942	956	rBV	1066658	1879734	24.43%	2.817%
9	8.981	1010	1019	1036	rBV	829865	1445774	18.79%	2.167%
10	9.699	1134	1141	1156	rBV	669573	1181145	15.35%	1.770%
11	10.240	1224	1233	1249	rBV	1059575	1919872	24.96%	2.877%
12	10.616	1288	1297	1313	rBV	1132014	1998131	25.97%	2.995%
13	10.763	1313	1322	1352	rBV	1141445	2253526	29.29%	3.377%
14	12.216	1560	1569	1575	rBV2	15549	35922	0.47%	0.054%
15	13.357	1757	1763	1768	rBV9	5811	8709	0.11%	0.013%
16	13.875	1844	1851	1864	rBV	2058087	2952682	38.38%	4.425%
17	13.969	1864	1867	1872	rVB7	4632	8580	0.11%	0.013%
18	14.151	1889	1898	1918	rBV	2441706	3727274	48.45%	5.586%
19	14.463	1942	1951	1966	rBV	1900369	2871006	37.32%	4.303%
20	14.681	1981	1988	2010	rBV	769580	1484665	19.30%	2.225%
21	15.457	2112	2120	2133	rBV	3242342	4734171	61.54%	7.095%
22	15.592	2137	2143	2157	rVV	888868	1317560	17.13%	1.975%
23	15.698	2157	2161	2167	rVB4	18292	32366	0.42%	0.049%
24	17.010	2381	2384	2389	rBV7	5385	9292	0.12%	0.014%
25	17.222	2413	2420	2429	rBV	2547863	3551941	46.17%	5.323%
26	17.322	2430	2437	2452	rVV	3849295	5528355	71.86%	8.286%
27	19.139	2742	2746	2751	rBV2	49579	66656	0.87%	0.100%
28	19.210	2754	2758	2764	rVV2	44159	65605	0.85%	0.098%
29	19.563	2812	2818	2831	rBV	5099750	6837578	88.88%	10.248%
30	21.316	3111	3116	3125	rBV	3473338	4484788	58.30%	6.722%
31	23.563	3491	3498	3513	rVB2	3715219	7692991	100.00%	11.530%
32	23.716	3518	3524	3534	rVB2	2175304	4416360	57.41%	6.619%
33	27.980	4245	4249	4251	rBV3	230934	391201	5.09%	0.586%


Sum of corrected areas: 66722274

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012340.D
Acq On : 27 Oct 2022 12:36
Operator : CG/JU
Sample : PB148454BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK454

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

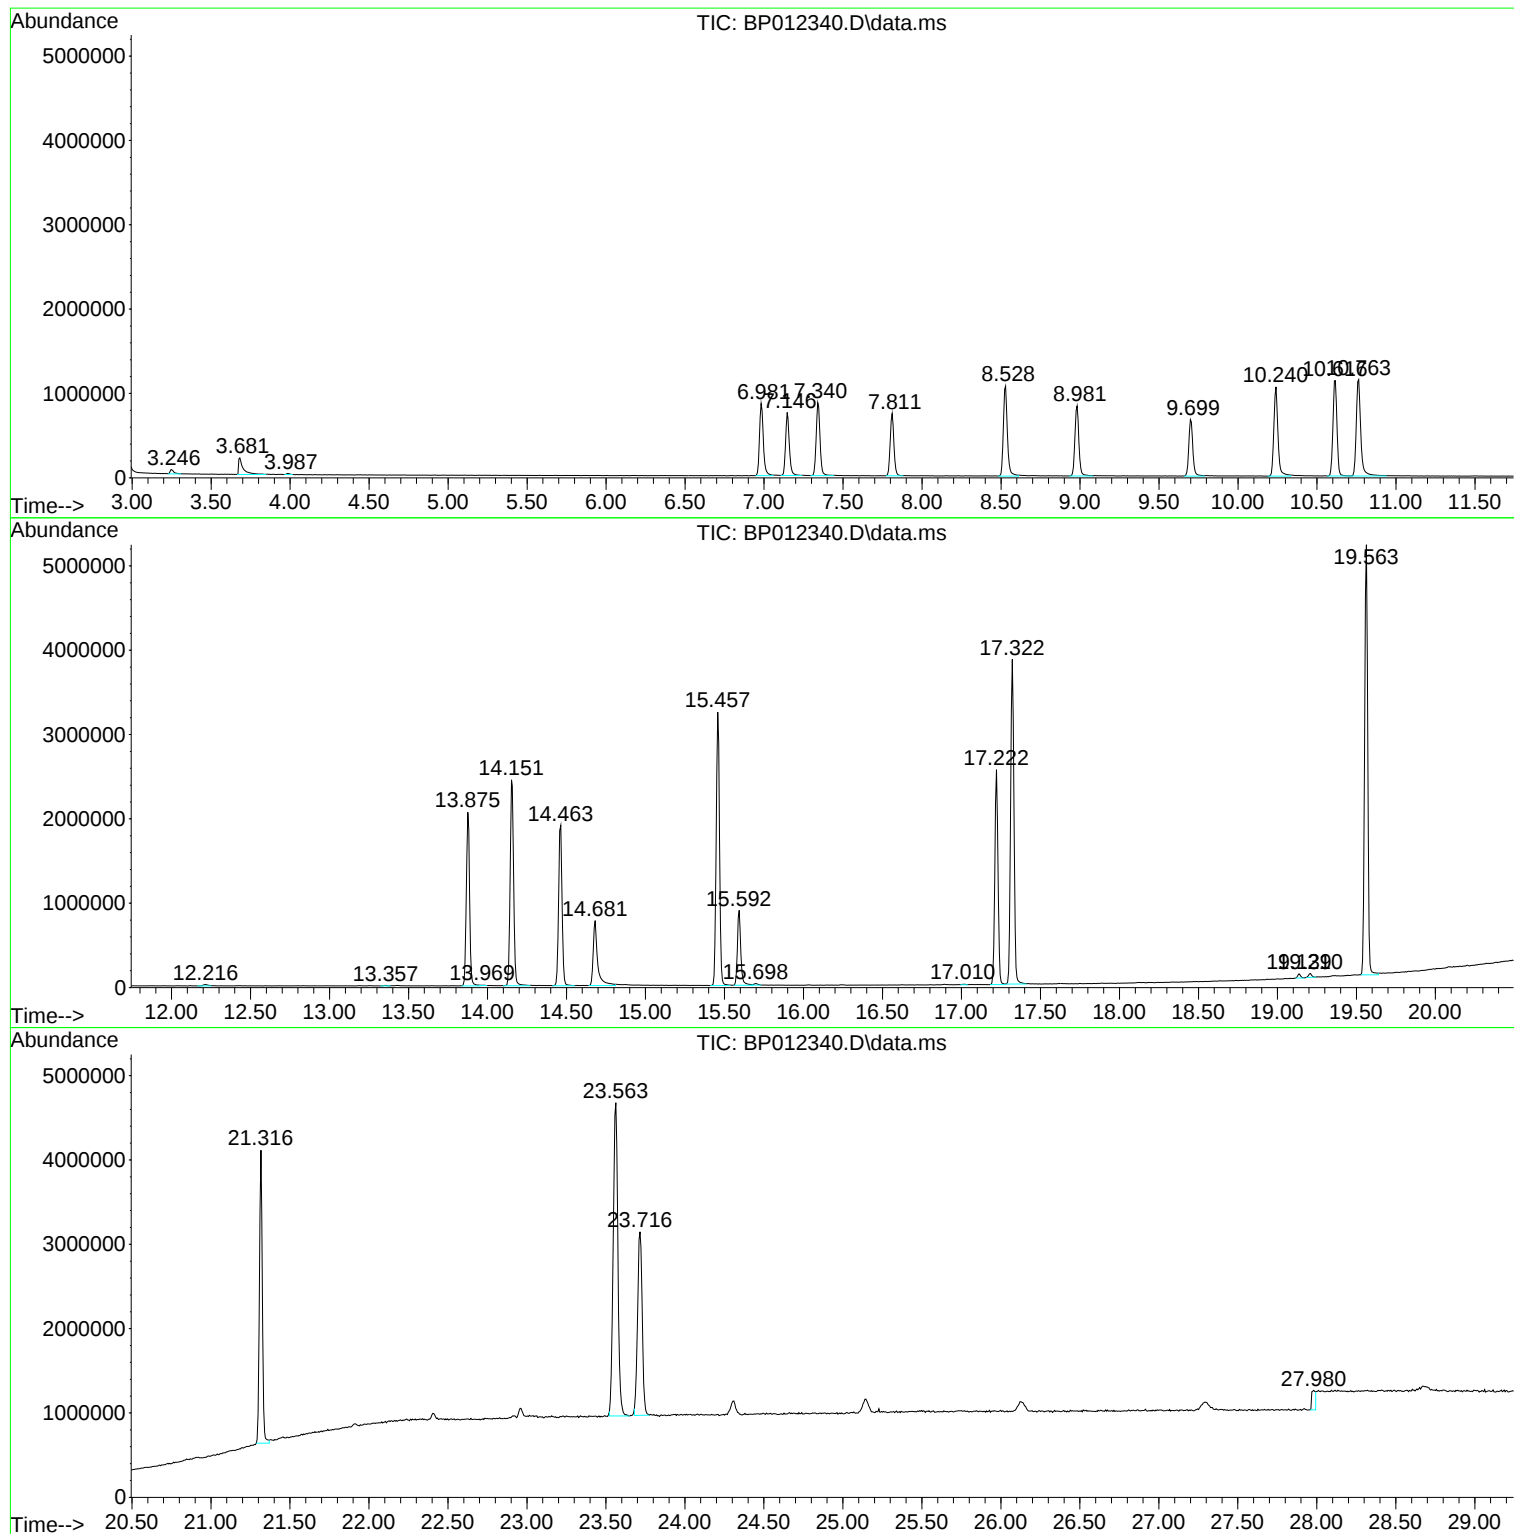

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012340.D
Acq On : 27 Oct 2022 12:36
Operator : CG/JU
Sample : PB148454BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK454

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012340.D
Acq On : 27 Oct 2022 12:36
Operator : CG/JU
Sample : PB148454BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK454

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc