

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012349.D
 Acq On : 27 Oct 2022 18:57
 Operator : CG/JU
 Sample : PB148403BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK403

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	54	rVB	74389	113972	1.22%	0.124%
2	3.670	113	116	138	rBV	596926	1051933	11.25%	1.142%
3	3.987	166	170	178	rVB2	18514	28293	0.30%	0.031%
4	6.981	672	679	700	rBV	1180189	2002128	21.40%	2.174%
5	7.146	700	707	719	rBV	1030153	1680560	17.97%	1.825%
6	7.340	733	740	751	rBV	1228687	1994349	21.32%	2.165%
7	7.805	812	819	832	rBV	1126677	1862563	19.91%	2.022%
8	8.522	933	941	959	rBV	1513057	2626097	28.08%	2.851%
9	8.975	1011	1018	1035	rBV	1207906	2055939	21.98%	2.232%
10	9.699	1133	1141	1155	rBV	1000134	1705290	18.23%	1.852%
11	10.234	1224	1232	1251	rBV	1531451	2733285	29.22%	2.968%
12	10.610	1287	1296	1313	rBV	1739335	3003122	32.11%	3.261%
13	10.757	1315	1321	1342	rBV	937004	1780262	19.03%	1.933%
14	12.216	1560	1569	1576	rBV2	20330	44783	0.48%	0.049%
15	13.187	1728	1734	1739	rBV7	4249	10636	0.11%	0.012%
16	13.345	1756	1761	1768	rBV7	7219	12548	0.13%	0.014%
17	13.875	1844	1851	1866	rBV	3058887	4358028	46.59%	4.732%
18	14.151	1889	1898	1919	rBV	3666004	5419037	57.93%	5.884%
19	14.457	1943	1950	1961	rBV	2974693	4438159	47.45%	4.819%
20	14.675	1981	1987	2008	rBV	1231400	2205595	23.58%	2.395%
21	14.869	2018	2020	2029	rVB10	8828	15162	0.16%	0.016%
22	15.457	2113	2120	2133	rBV	4694516	6876228	73.51%	7.466%
23	15.587	2136	2142	2156	rVV	1294195	1980759	21.18%	2.151%
24	15.698	2156	2161	2169	rVB	27761	54865	0.59%	0.060%
25	17.010	2380	2384	2391	rVB5	6979	11519	0.12%	0.013%
26	17.222	2413	2420	2430	rBV	3669460	5485273	58.64%	5.956%
27	17.322	2430	2437	2452	rVV2	5124483	7760189	82.96%	8.426%
28	17.892	2530	2534	2537	rVB5	7838	11489	0.12%	0.012%
29	18.110	2568	2571	2578	rBV7	19586	34475	0.37%	0.037%
30	18.386	2615	2618	2623	rVB5	12971	13795	0.15%	0.015%
31	19.133	2742	2745	2751	rBV	68937	93200	1.00%	0.101%
32	19.204	2753	2757	2762	rBV	65419	92470	0.99%	0.100%
33	19.563	2812	2818	2827	rBV	6774940	9353835	100.00%	10.157%
34	21.316	3111	3116	3126	rBV	4868104	6414638	68.58%	6.965%
35	23.557	3490	3497	3511	rVB2	4426062	9002255	96.24%	9.775%
36	23.710	3517	3523	3534	rVB2	2839248	5770063	61.69%	6.265%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012349.D
Acq On : 27 Oct 2022 18:57
Operator : CG/JU
Sample : PB148403BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK403

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 92096794

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012349.D
Acq On : 27 Oct 2022 18:57
Operator : CG/JU
Sample : PB148403BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK403

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

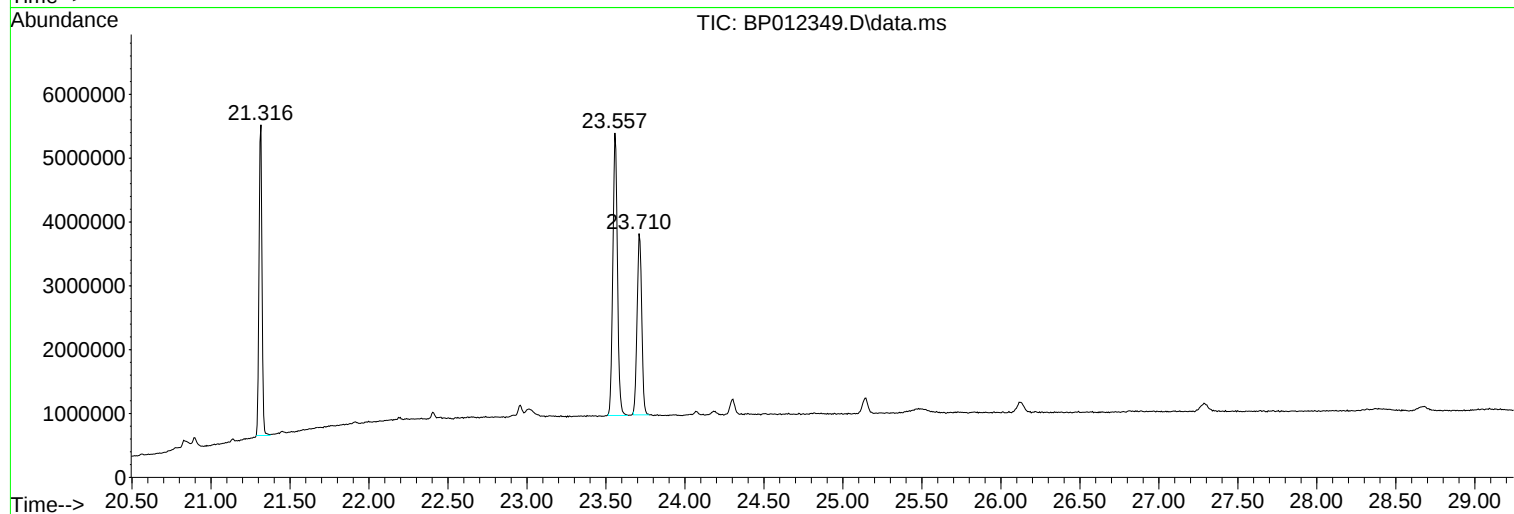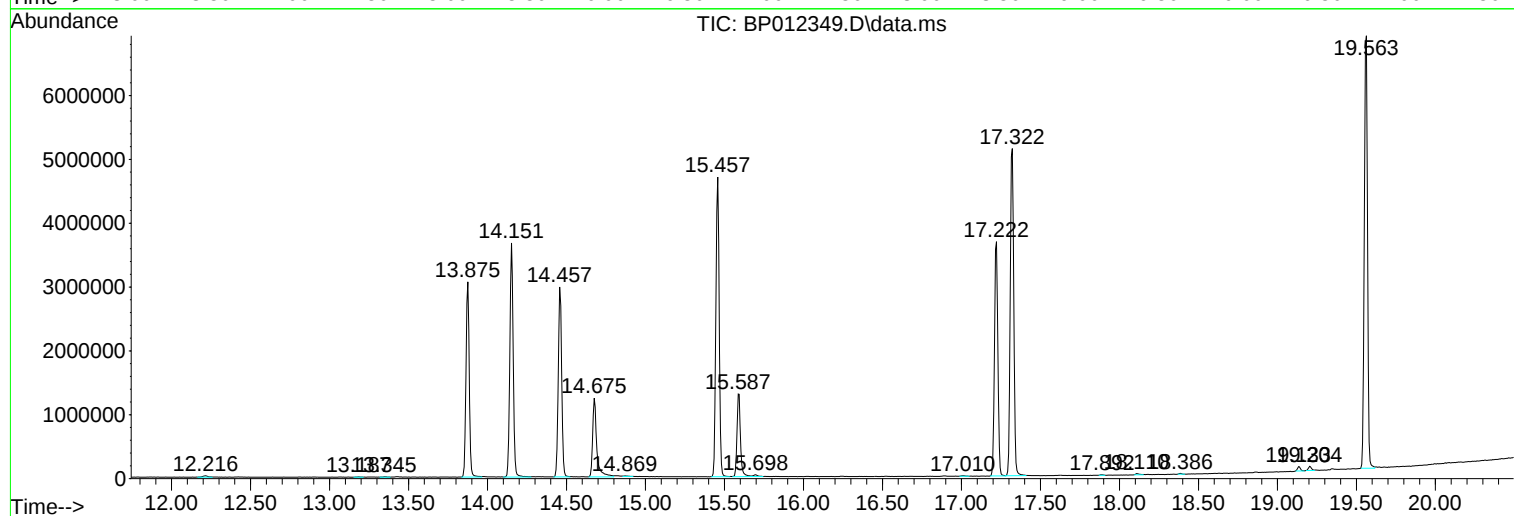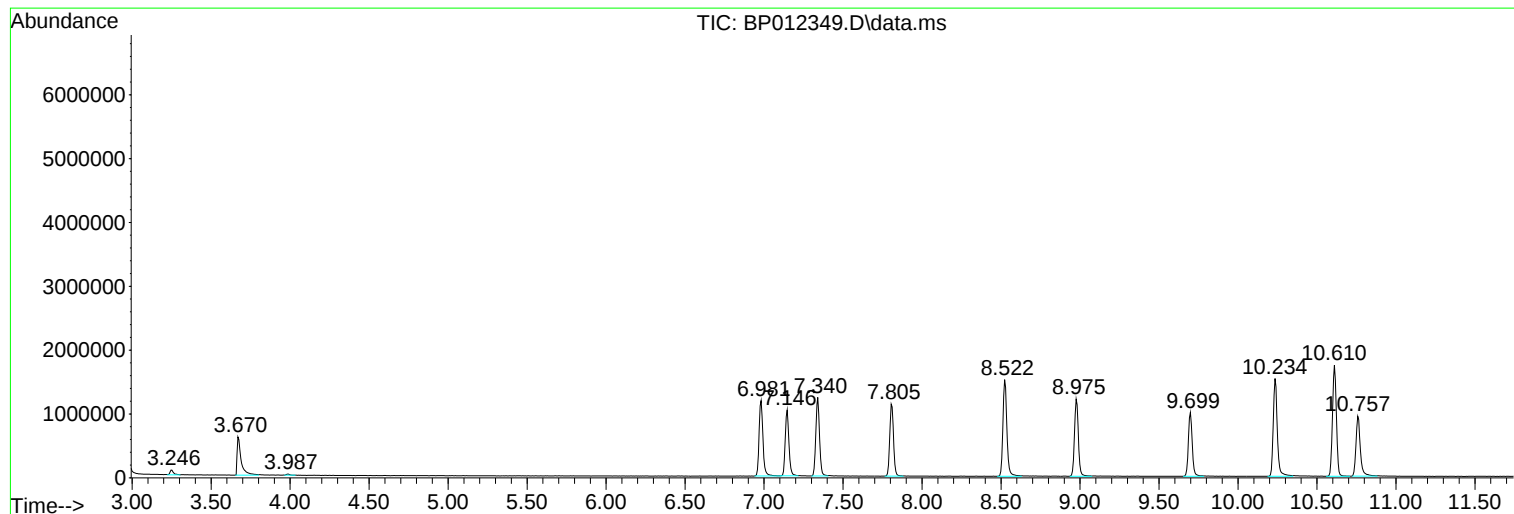

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012349.D
Acq On : 27 Oct 2022 18:57
Operator : CG/JU
Sample : PB148403BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK403

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012349.D
Acq On : 27 Oct 2022 18:57
Operator : CG/JU
Sample : PB148403BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK403

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc