

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012367.D
 Acq On : 28 Oct 2022 08:58
 Operator : CG/JU
 Sample : PB148502BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK502

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	50	rBV	55182	75657	0.85%	0.101%
2	3.681	117	118	138	rBV	97698	201947	2.26%	0.270%
3	3.981	166	169	176	rVB	14332	21886	0.25%	0.029%
4	6.981	672	679	697	rBV	980314	1626523	18.21%	2.172%
5	7.146	700	707	719	rBV	822753	1331047	14.90%	1.777%
6	7.340	733	740	756	rBV	987998	1609641	18.02%	2.149%
7	7.811	813	820	830	rBV	795305	1287952	14.42%	1.720%
8	8.528	932	942	962	rBV	1206986	2158252	24.17%	2.882%
9	8.981	1011	1019	1034	rBV	1010384	1654010	18.52%	2.208%
10	9.699	1131	1141	1155	rBV	782321	1365899	15.29%	1.824%
11	10.240	1225	1233	1251	rBV	1203457	2222627	24.89%	2.968%
12	10.616	1288	1297	1314	rBV	1251355	2140002	23.96%	2.857%
13	12.210	1561	1568	1577	rBV	20711	46178	0.52%	0.062%
14	13.434	1770	1776	1780	rBV7	5659	10585	0.12%	0.014%
15	13.881	1845	1852	1865	rBV	2416452	3544992	39.69%	4.733%
16	14.157	1892	1899	1918	rBV	2961340	4455746	49.89%	5.949%
17	14.463	1944	1951	1964	rBV	2119544	3216302	36.01%	4.294%
18	14.681	1982	1988	2012	rBV	1046892	1912348	21.41%	2.553%
19	15.463	2114	2121	2135	rVB	3998436	5747004	64.35%	7.673%
20	15.593	2137	2143	2157	rVV	1034820	1555487	17.42%	2.077%
21	15.704	2157	2162	2167	rVB	20470	35262	0.39%	0.047%
22	15.975	2204	2208	2211	rBV6	5767	9342	0.10%	0.012%
23	16.257	2251	2256	2262	rBV9	6141	12201	0.14%	0.016%
24	17.228	2414	2421	2431	rBV	2914722	4140551	46.36%	5.528%
25	17.328	2431	2438	2456	rVV	4735833	6577564	73.65%	8.782%
26	18.116	2569	2572	2579	rBV7	12678	18895	0.21%	0.025%
27	19.145	2743	2747	2751	rBV3	59148	83231	0.93%	0.111%
28	19.210	2755	2758	2764	rVB	49117	70849	0.79%	0.095%
29	19.569	2813	2819	2825	rBV	6289746	8217007	92.01%	10.971%
30	21.322	3112	3117	3128	rBV	4219189	5399638	60.46%	7.209%
31	23.569	3492	3499	3510	rVB	4508992	8930950	100.00%	11.924%
32	23.722	3519	3525	3536	rVB2	2601694	5217893	58.42%	6.967%




Sum of corrected areas: 74897468

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012367.D
Acq On : 28 Oct 2022 08:58
Operator : CG/JU
Sample : PB148502BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

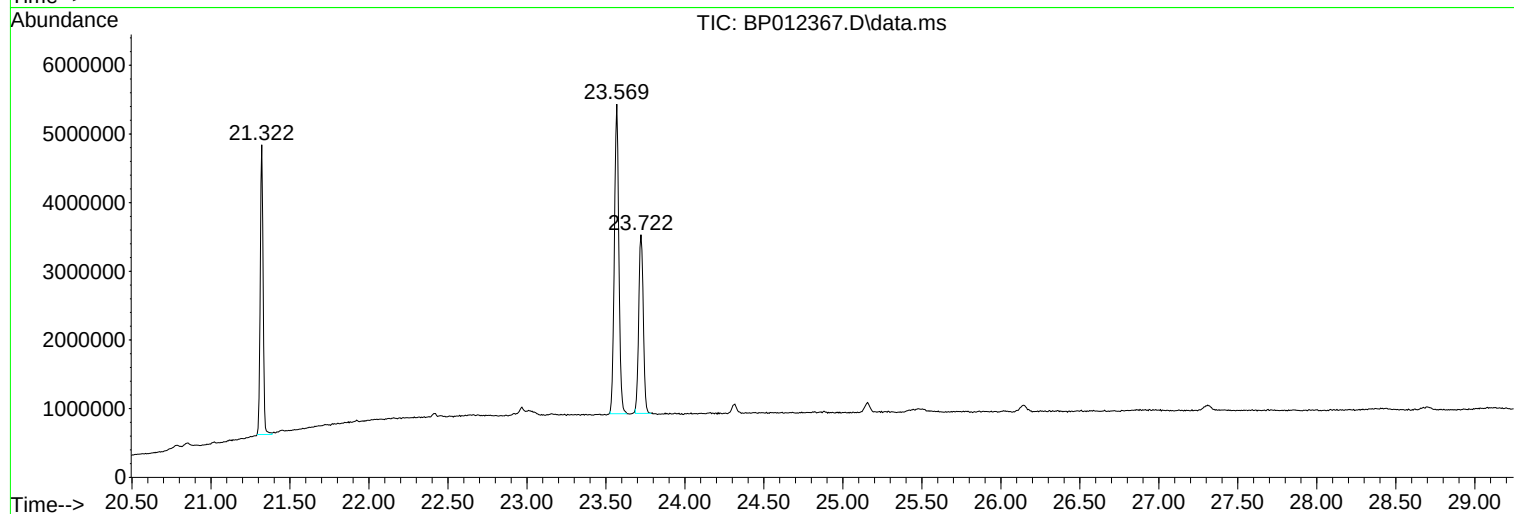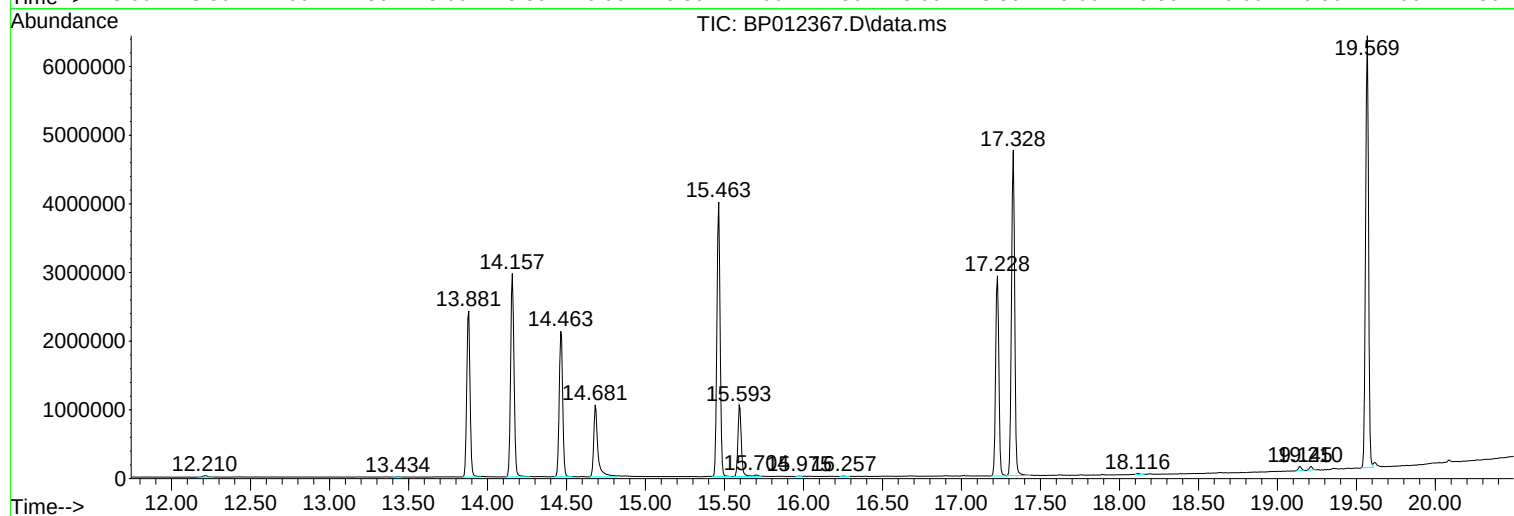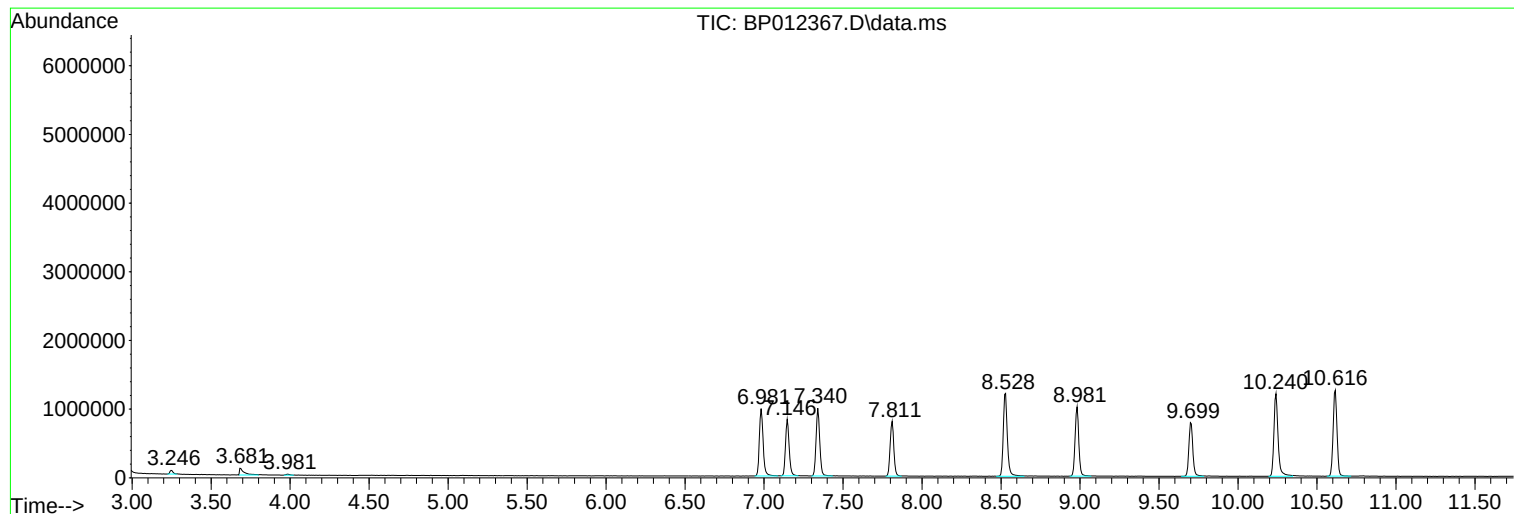

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012367.D
Acq On : 28 Oct 2022 08:58
Operator : CG/JU
Sample : PB148502BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012367.D
Acq On : 28 Oct 2022 08:58
Operator : CG/JU
Sample : PB148502BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------