

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012372.D
 Acq On : 28 Oct 2022 11:48
 Operator : CG/JU
 Sample : N5232-11
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	48	rBV	38243	52034	0.51%	0.063%
2	3.699	118	121	130	rBV	23100	52379	0.51%	0.064%
3	3.887	148	153	160	rBV	29775	49972	0.49%	0.061%
4	3.981	166	169	179	rVB	18143	29450	0.29%	0.036%
5	4.358	230	233	239	rVB6	6936	11525	0.11%	0.014%
6	5.116	354	362	370	rBV	66188	107576	1.04%	0.131%
7	6.981	673	679	690	rBV	209196	381723	3.71%	0.465%
8	7.140	698	706	720	rBV	866557	1460956	14.19%	1.778%
9	7.334	733	739	758	rVB	805012	1355163	13.16%	1.649%
10	7.805	809	819	833	rBV	885660	1468965	14.27%	1.788%
11	8.005	849	853	856	rVB4	9243	13583	0.13%	0.017%
12	8.163	873	880	884	rBV8	10190	21072	0.20%	0.026%
13	8.522	934	941	956	rBV	690987	1228616	11.93%	1.495%
14	8.975	1010	1018	1031	rBV	1074911	1818111	17.66%	2.213%
15	9.093	1035	1038	1054	rVB6	16542	59999	0.58%	0.073%
16	9.252	1061	1065	1070	rVB4	7216	10964	0.11%	0.013%
17	9.357	1080	1083	1090	rVB4	13525	22628	0.22%	0.028%
18	9.693	1132	1140	1153	rBV	819908	1408587	13.68%	1.715%
19	9.793	1155	1157	1164	rVV7	9618	14383	0.14%	0.018%
20	10.028	1193	1197	1204	rVB7	5855	12525	0.12%	0.015%
21	10.234	1224	1232	1253	rBV	1285869	2332774	22.66%	2.839%
22	10.399	1254	1260	1284	rVV	111710	321862	3.13%	0.392%
23	10.604	1287	1295	1309	rVV	1323057	2306088	22.40%	2.807%
24	10.763	1316	1322	1333	rVB	78650	175155	1.70%	0.213%
25	11.069	1370	1374	1383	rVB8	6163	13005	0.13%	0.016%
26	11.187	1389	1394	1397	rBV5	7533	12751	0.12%	0.016%
27	11.298	1408	1413	1421	rVB10	4195	11341	0.11%	0.014%
28	11.434	1431	1436	1444	rBV10	5352	16136	0.16%	0.020%
29	11.510	1444	1449	1456	rVB10	5875	13131	0.13%	0.016%
30	11.963	1518	1526	1533	rBV	35242	68184	0.66%	0.083%
31	12.175	1553	1562	1563	rBV3	13686	23730	0.23%	0.029%
32	12.204	1563	1567	1574	rVB2	21829	41264	0.40%	0.050%
33	12.569	1623	1629	1631	rBV4	7923	11048	0.11%	0.013%
34	12.710	1647	1653	1661	rBV4	7473	21209	0.21%	0.026%
35	12.992	1697	1701	1706	rBV2	10547	19026	0.18%	0.023%
36	13.269	1740	1748	1752	rBV4	13371	24761	0.24%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012372.D
 Acq On : 28 Oct 2022 11:48
 Operator : CG/JU
 Sample : N5232-11
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	13.345	1756	1761	1767	rBV3	43603	72936	0.71%	0.089%
38	13.422	1770	1774	1780	rBV9	7132	13316	0.13%	0.016%
39	13.869	1842	1850	1863	rBV	2949056	4258718	41.37%	5.184%
40	14.151	1885	1898	1911	rBV	3276479	5109307	49.63%	6.219%
41	14.251	1913	1915	1924	rVB8	12087	23377	0.23%	0.028%
42	14.457	1942	1950	1967	rVB	2184889	3356837	32.61%	4.086%
43	14.687	1982	1989	2005	rBV	184587	427149	4.15%	0.520%
44	14.839	2012	2015	2018	rBV2	11015	13914	0.14%	0.017%
45	14.987	2036	2040	2047	rVB8	9125	18022	0.18%	0.022%
46	15.204	2073	2077	2082	rBV	43273	58974	0.57%	0.072%
47	15.245	2082	2084	2088	rVV4	8069	11863	0.12%	0.014%
48	15.286	2088	2091	2096	rVB4	10840	18778	0.18%	0.023%
49	15.451	2113	2119	2126	rBV	4450227	6723061	65.30%	8.183%
50	15.586	2135	2142	2154	rBV	1462186	2054854	19.96%	2.501%
51	15.681	2154	2158	2171	rVB2	51335	121053	1.18%	0.147%
52	15.816	2177	2181	2186	rVB7	13399	24231	0.24%	0.029%
53	15.975	2202	2208	2213	rBV	63100	94335	0.92%	0.115%
54	16.157	2232	2239	2248	rBV	211964	403058	3.92%	0.491%
55	16.492	2292	2296	2305	rBV	35157	59223	0.58%	0.072%
56	17.028	2384	2387	2393	rVB3	16493	22123	0.21%	0.027%
57	17.216	2413	2419	2429	rBV	2977831	4225349	41.04%	5.143%
58	17.316	2429	2436	2448	rBV2	5531020	8019539	77.90%	9.761%
59	17.845	2524	2526	2529	rBV2	16229	19686	0.19%	0.024%
60	17.880	2529	2532	2540	rVB	81585	106288	1.03%	0.129%
61	18.098	2565	2569	2579	rBV	199587	337824	3.28%	0.411%
62	19.133	2741	2745	2749	rVB2	79677	107708	1.05%	0.131%
63	19.198	2752	2756	2765	rBV	93327	163472	1.59%	0.199%
64	19.333	2776	2779	2786	rBV	183787	269230	2.62%	0.328%
65	19.557	2811	2817	2823	rBV	7592949	10203541	99.11%	12.420%
66	21.021	3063	3066	3073	rVB3	158328	224865	2.18%	0.274%
67	21.310	3110	3115	3121	rBV	4281188	5400561	52.46%	6.573%
68	23.551	3489	3496	3509	rVB2	5096487	10295211	100.00%	12.531%
69	23.704	3516	3522	3533	rVB2	2413436	4906852	47.66%	5.973%




Sum of corrected areas: 82156931

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012372.D
Acq On : 28 Oct 2022 11:48
Operator : CG/JU
Sample : N5232-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

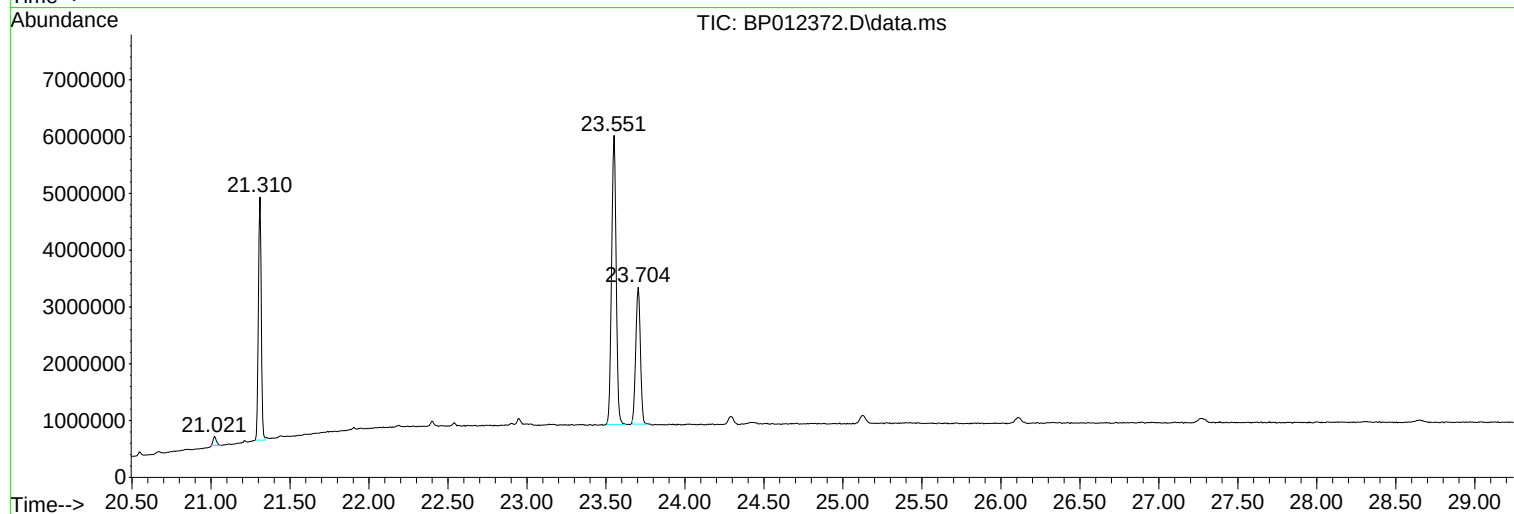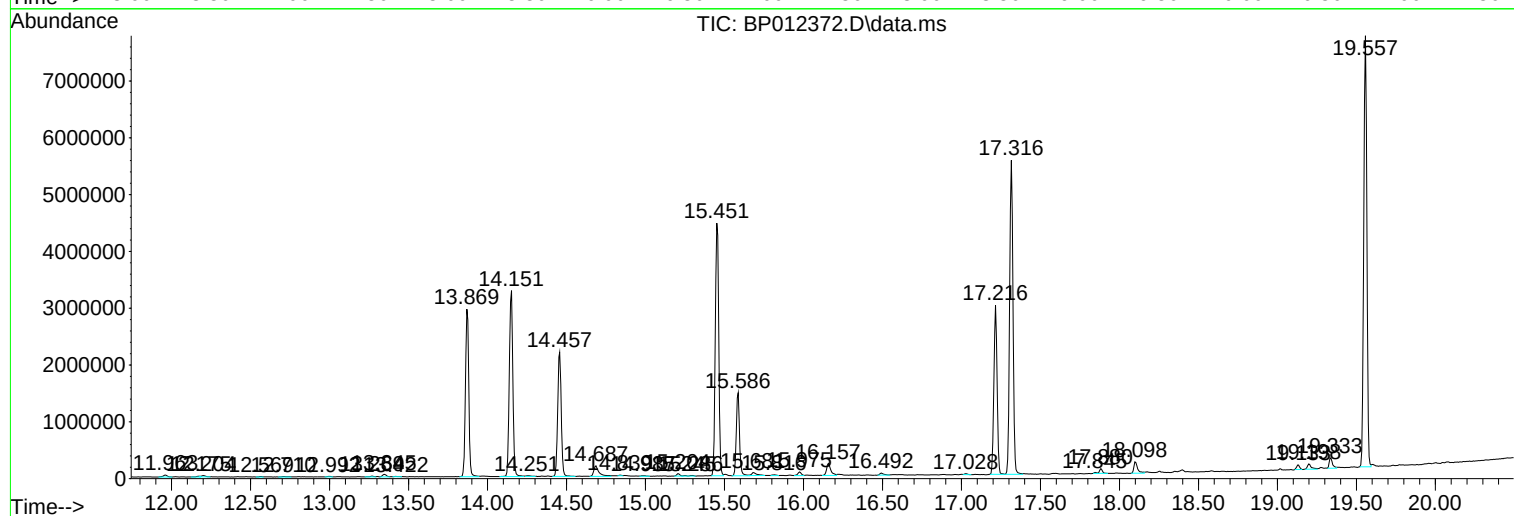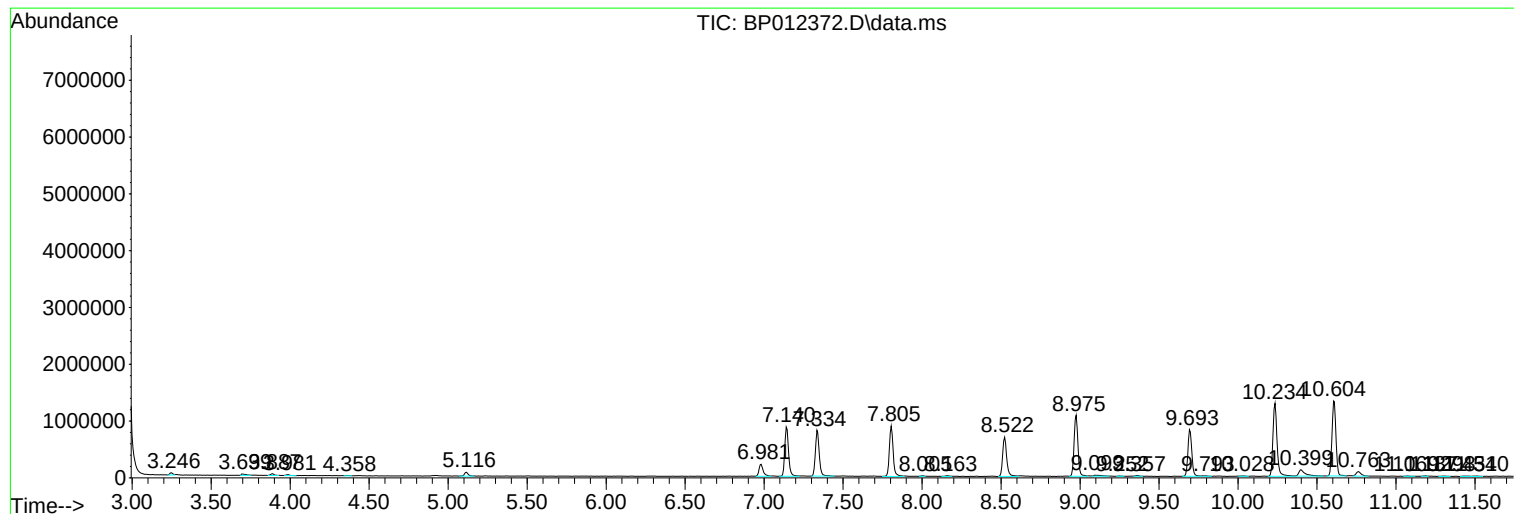

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012372.D
Acq On : 28 Oct 2022 11:48
Operator : CG/JU
Sample : N5232-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA65










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 1-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.399	2.79 ng/ul	321862	Naphthalene-d8	10.604

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	78
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72
5			Ethylene glycol monoisobutyl ether	118	C6H14O2	004439-24-1	64

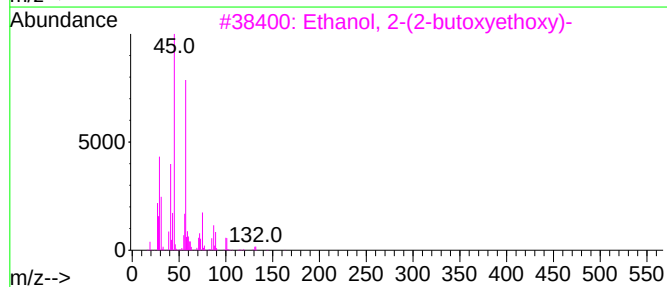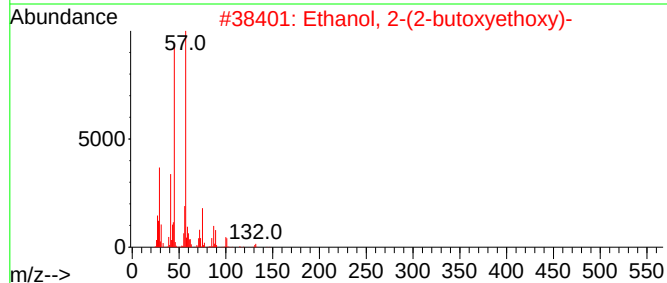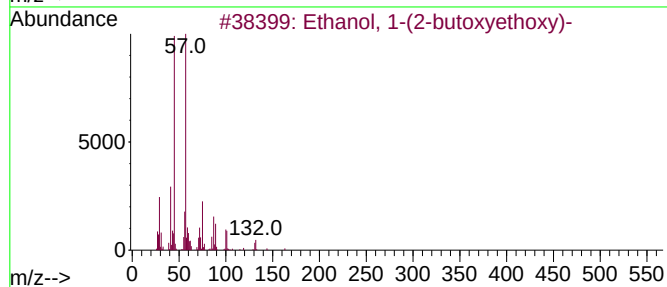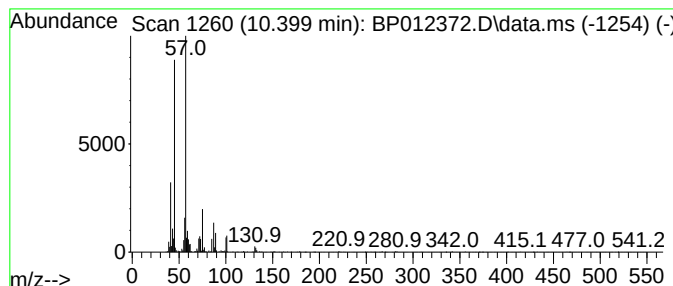

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012372.D
Acq On : 28 Oct 2022 11:48
Operator : CG/JU
Sample : N5232-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 1-(2-b...	10.399	2.8	ng/u1	321862	2	10.604	2306090	20.0