

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012374.D
 Acq On : 28 Oct 2022 12:57
 Operator : CG/JU
 Sample : N5232-14
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	52	rVB	42912	64691	0.63%	0.085%
2	3.693	119	120	128	rBV	27156	51255	0.50%	0.067%
3	3.887	147	153	158	rBV	37524	63856	0.62%	0.084%
4	3.981	166	169	177	rVB	17335	26328	0.26%	0.035%
5	5.116	358	362	366	rVB2	12627	17545	0.17%	0.023%
6	6.981	672	679	690	rBV	231737	423825	4.13%	0.557%
7	7.140	700	706	719	rBV	926439	1544704	15.04%	2.029%
8	7.334	732	739	750	rBV	868025	1453937	14.15%	1.910%
9	7.804	811	819	833	rBV	776204	1272199	12.38%	1.671%
10	8.210	884	888	895	rBV7	6138	11117	0.11%	0.015%
11	8.522	934	941	953	rBV	720987	1253767	12.20%	1.647%
12	8.975	1010	1018	1036	rBV	1101685	1910863	18.60%	2.510%
13	9.357	1078	1083	1089	rVB4	10820	20954	0.20%	0.028%
14	9.692	1132	1140	1155	rBV	880236	1535570	14.95%	2.017%
15	10.234	1225	1232	1251	rBV	1267331	2286462	22.26%	3.003%
16	10.410	1256	1262	1275	rVV2	19408	66577	0.65%	0.087%
17	10.604	1287	1295	1308	rBV	1172587	2024424	19.70%	2.659%
18	10.763	1314	1322	1336	rVB	99796	220457	2.15%	0.290%
19	11.304	1408	1414	1421	rVB2	13237	25545	0.25%	0.034%
20	12.204	1561	1567	1574	rBV2	22999	43300	0.42%	0.057%
21	12.986	1694	1700	1706	rBV4	17937	36914	0.36%	0.048%
22	13.269	1742	1748	1752	rVV2	9326	14698	0.14%	0.019%
23	13.345	1757	1761	1767	rVB6	10840	18482	0.18%	0.024%
24	13.422	1770	1774	1778	rVB7	7685	10411	0.10%	0.014%
25	13.869	1843	1850	1864	rBV	2767712	3875642	37.72%	5.091%
26	13.963	1864	1866	1872	rVB7	5543	10564	0.10%	0.014%
27	14.151	1887	1898	1908	rBV	3179417	4904768	47.74%	6.443%
28	14.457	1941	1950	1968	rBV	1963059	2962433	28.83%	3.891%
29	14.686	1983	1989	2002	rBV2	139796	350267	3.41%	0.460%
30	15.080	2053	2056	2063	rVB4	8870	12071	0.12%	0.016%
31	15.210	2072	2078	2082	rBV	165452	234851	2.29%	0.308%
32	15.286	2088	2091	2099	rVB4	11582	23621	0.23%	0.031%
33	15.451	2112	2119	2132	rBV	4426709	6274328	61.07%	8.242%
34	15.586	2136	2142	2151	rBV	1209122	1727995	16.82%	2.270%
35	15.692	2156	2160	2172	rVB2	25062	46374	0.45%	0.061%
36	15.969	2203	2207	2212	rBV3	20145	32920	0.32%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
 Data File : BP012374.D
 Acq On : 28 Oct 2022 12:57
 Operator : CG/JU
 Sample : N5232-14
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	16.104	2225	2230	2235	rBV	13554	20291	0.20%	0.027%
38	16.510	2295	2299	2303	rBV7	5852	11974	0.12%	0.016%
39	16.604	2310	2315	2316	rBV4	6867	10372	0.10%	0.014%
40	16.892	2359	2364	2371	rBV4	9356	20312	0.20%	0.027%
41	17.216	2412	2419	2429	rBV	2648988	3742603	36.43%	4.916%
42	17.315	2429	2436	2453	rVV2	4922171	7370713	71.74%	9.682%
43	17.880	2529	2532	2536	rBV	34917	44934	0.44%	0.059%
44	18.104	2566	2570	2577	rBV2	69456	110839	1.08%	0.146%
45	19.133	2741	2745	2750	rBV	72305	104009	1.01%	0.137%
46	19.204	2753	2757	2768	rVB	75617	131470	1.28%	0.173%
47	19.339	2777	2780	2785	rBV5	53086	69142	0.67%	0.091%
48	19.557	2811	2817	2831	rBV	7126892	9489910	92.37%	12.466%
49	21.309	3110	3115	3121	rBV	4019086	5049237	49.15%	6.633%
50	23.550	3489	3496	3510	rVB2	5034563	10273902	100.00%	13.495%
51	23.703	3516	3522	3537	rVB2	2381050	4825080	46.96%	6.338%




Sum of corrected areas: 76128503

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012374.D
Acq On : 28 Oct 2022 12:57
Operator : CG/JU
Sample : N5232-14
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA82

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

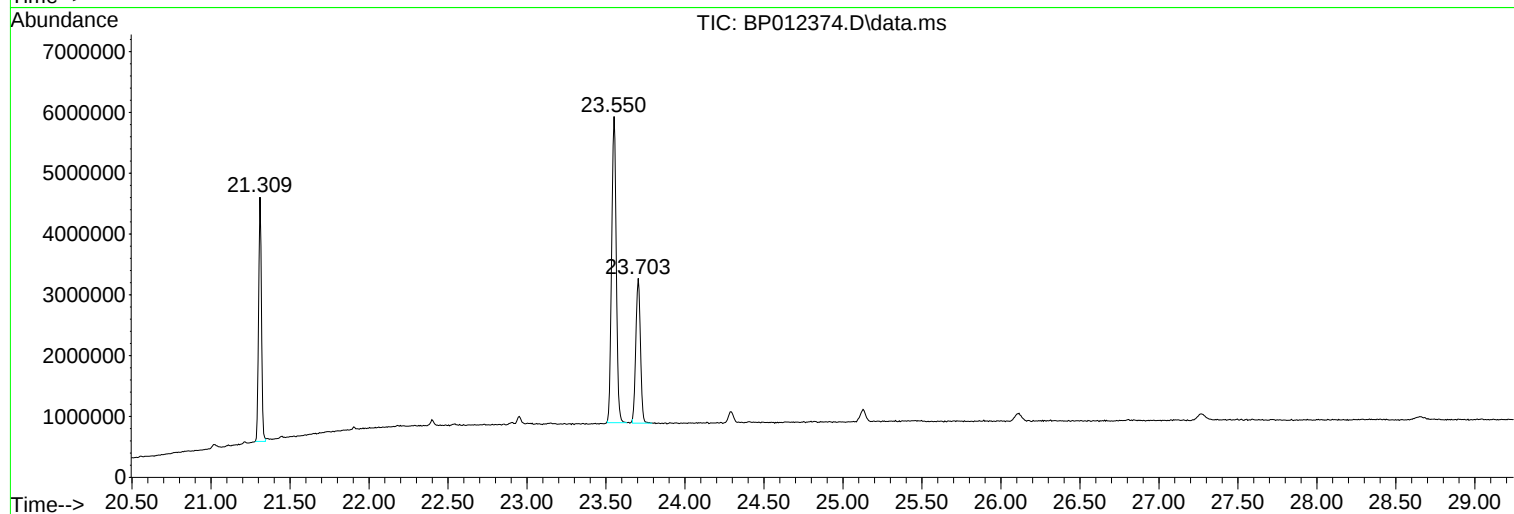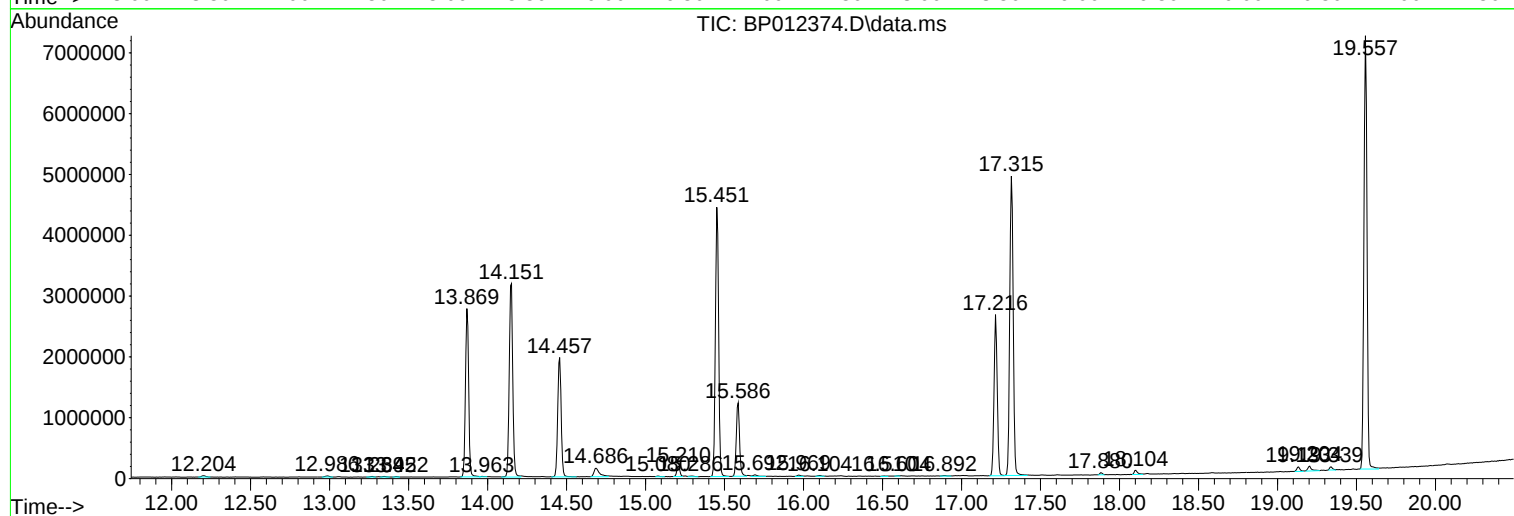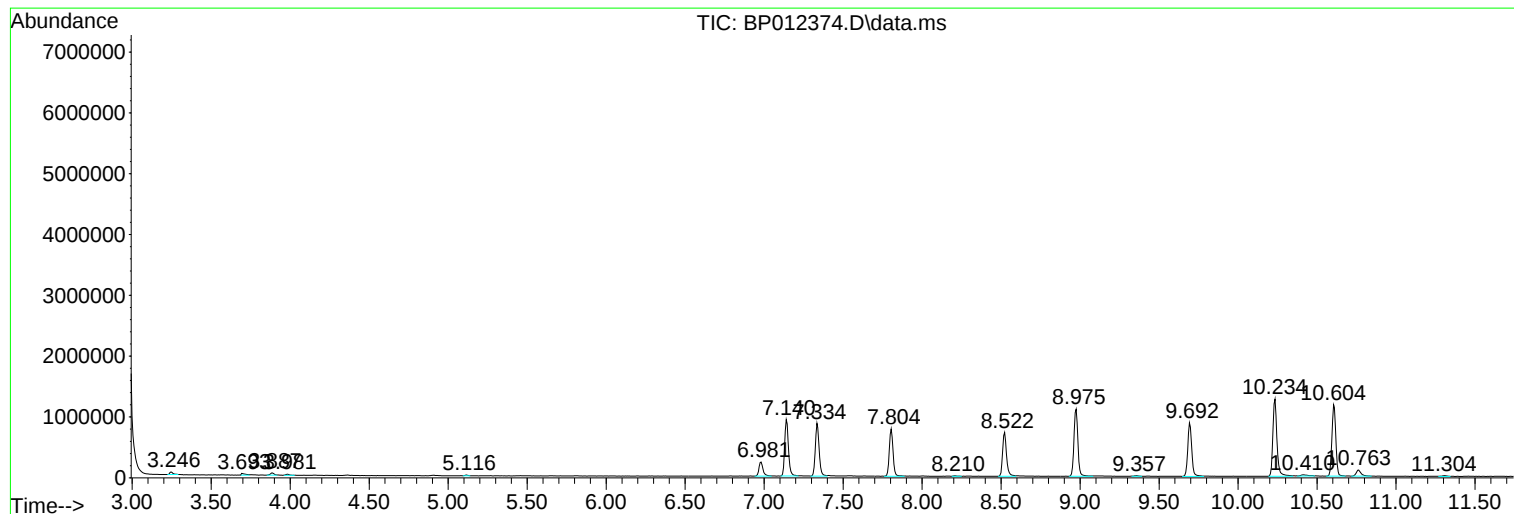

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012374.D
Acq On : 28 Oct 2022 12:57
Operator : CG/JU
Sample : N5232-14
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA82

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102722\
Data File : BP012374.D
Acq On : 28 Oct 2022 12:57
Operator : CG/JU
Sample : N5232-14
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA82

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc