
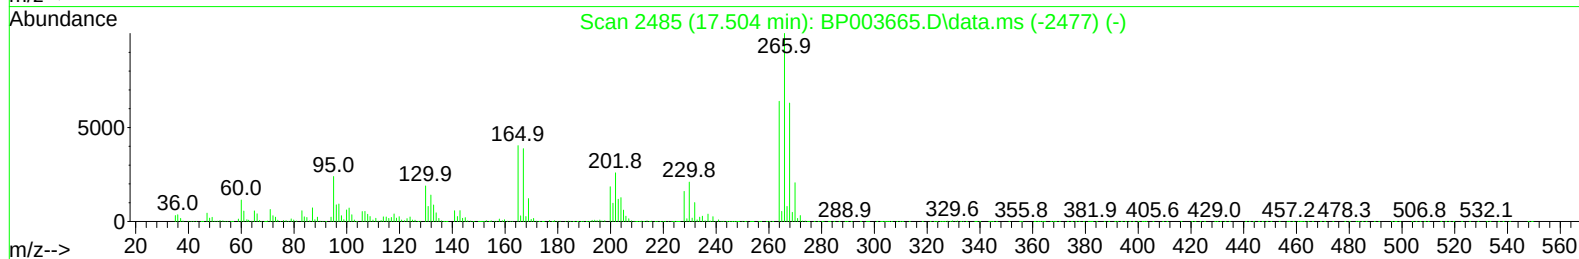
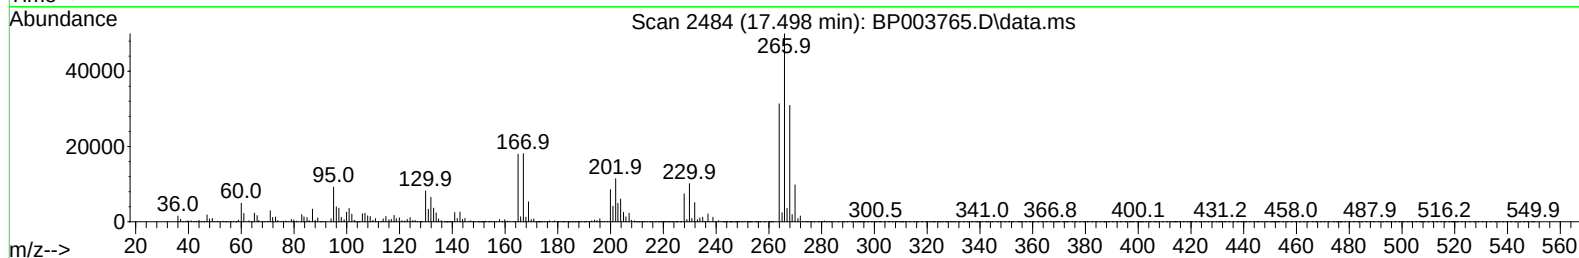


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102820\
Data File : BP003765.D
Acq On : 28 Oct 2020 09:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 01:53:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 16:22:21 2020
Response via : Initial Calibration

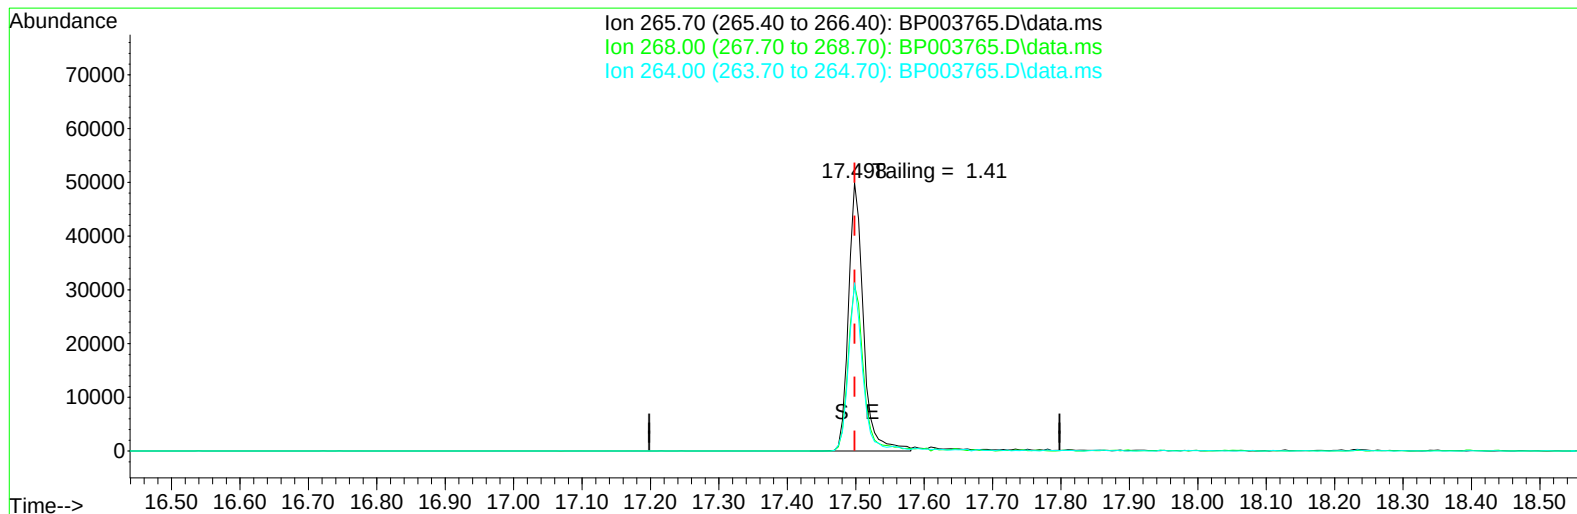

TIC: BP003765.D\data.ms

(70) Pentachlorophenol (C)




17.498min (-0.000) 250652.39 ng

response 74385

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.91
264.00	63.30	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102820\
Data File : BP003765.D
Acq On : 28 Oct 2020 09:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 01:53:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 16:22:21 2020
Response via : Initial Calibration

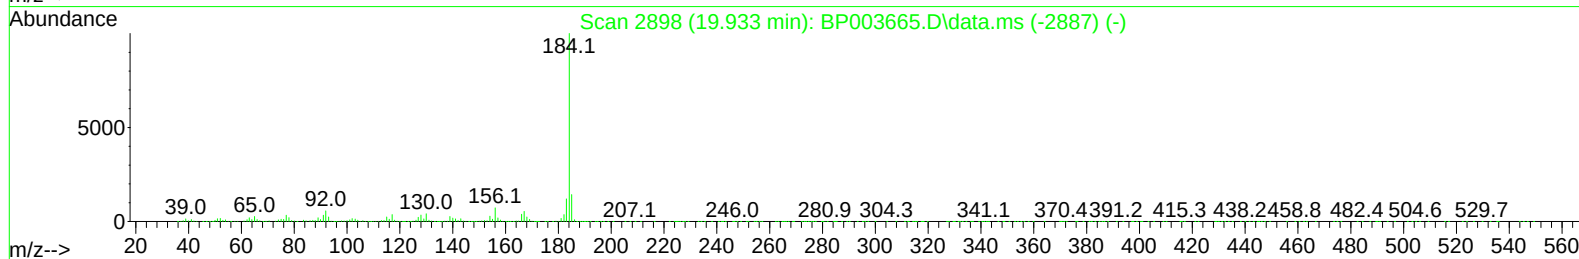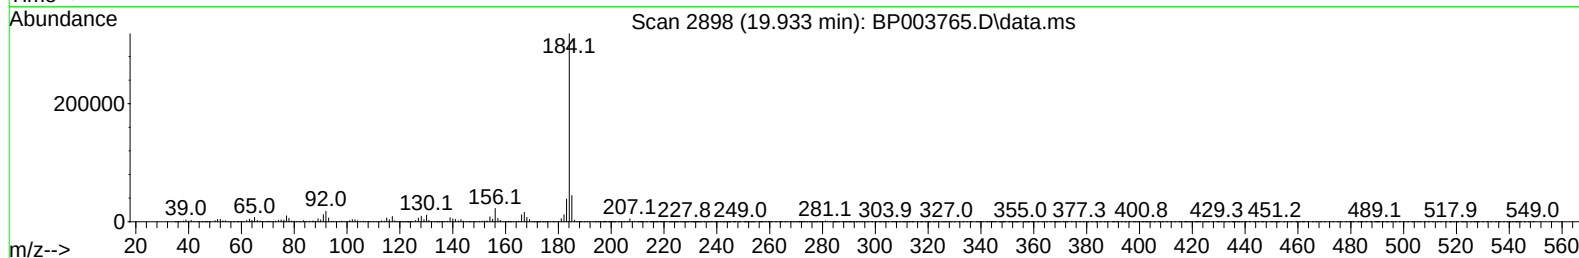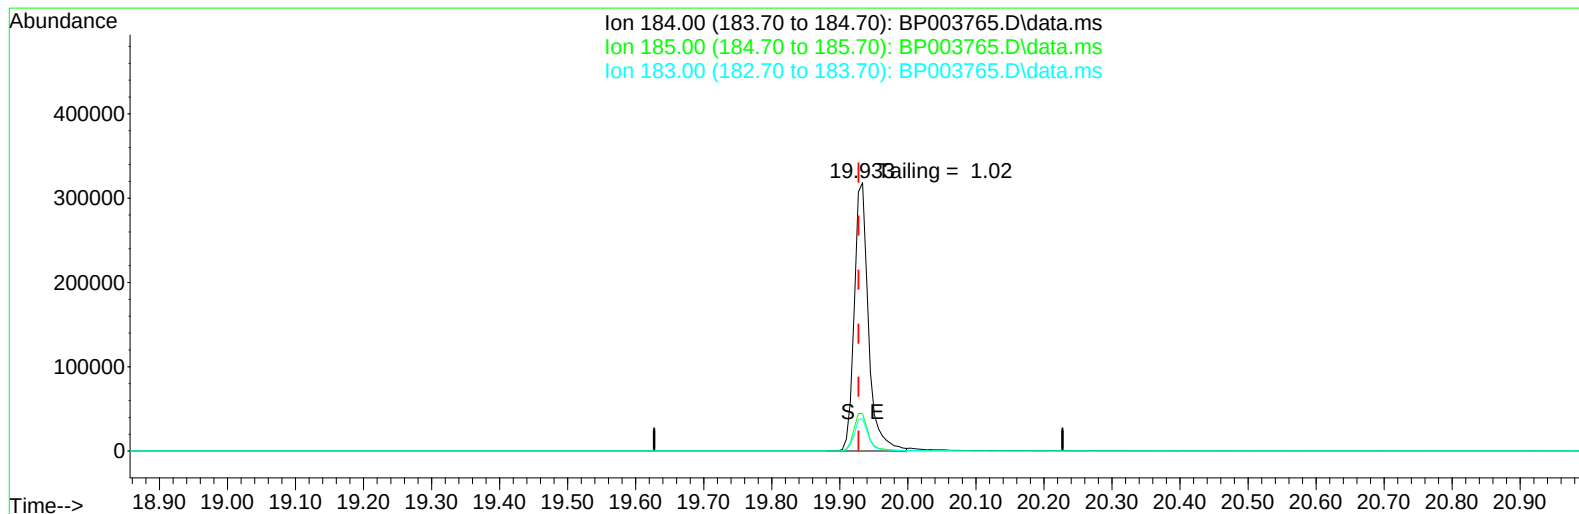

TIC: BP003765.D\data.ms

(77) Benzidine**19.933min (+ 0.006) 516113.31 ng****response 457548**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.94
183.00	12.00	12.06
0.00	0.00	0.00