

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102820\
 Data File : BP003767.D
 Acq On : 28 Oct 2020 13:09
 Operator : CG/JU
 Sample : PB132669BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132669BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.087	29	34	51	rVB	7379697	8644407	100.00%	18.257%
2	6.005	521	530	541	rBV	2313547	3493567	40.41%	7.379%
3	7.663	803	812	823	rBV	2088498	3448051	39.89%	7.282%
4	8.510	948	956	963	rBV	467560	751114	8.69%	1.586%
5	9.675	1146	1154	1162	rBV	1369365	2257277	26.11%	4.767%
6	11.351	1431	1439	1448	rBV	575724	979916	11.34%	2.070%
7	13.740	1837	1845	1859	rBV	3576610	5244599	60.67%	11.077%
8	15.116	2071	2079	2094	rBV	854917	1293825	14.97%	2.733%
9	16.587	2319	2329	2347	rBV	2855452	4226944	48.90%	8.927%
10	17.833	2534	2541	2554	rBV	1103127	1596461	18.47%	3.372%
11	18.175	2584	2599	2608	rBV3	32104	143231	1.66%	0.303%
12	18.333	2615	2626	2637	rBV3	57769	231867	2.68%	0.490%
13	18.457	2638	2647	2659	rVB	147608	392692	4.54%	0.829%
14	19.510	2820	2826	2835	rVB2	48721	97086	1.12%	0.205%
15	20.310	2956	2962	2971	rBV	7185741	8504940	98.39%	17.963%
16	20.404	2972	2978	2986	rVB	101842	189712	2.19%	0.401%
17	21.145	3099	3104	3110	rBV	197933	286336	3.31%	0.605%
18	21.310	3122	3132	3143	rVB	218877	507366	5.87%	1.072%
19	21.857	3216	3225	3233	rBV	1343256	2128606	24.62%	4.496%
20	22.592	3344	3350	3360	rVB	186977	368961	4.27%	0.779%
21	23.110	3434	3438	3445	rVB	185636	286859	3.32%	0.606%
22	23.416	3484	3490	3498	rVB2	131196	299877	3.47%	0.633%
23	23.527	3506	3509	3516	rVB3	67072	113907	1.32%	0.241%
24	24.192	3618	3622	3629	rVB	70245	118190	1.37%	0.250%
25	24.439	3657	3664	3675	rVB	842814	1741700	20.15%	3.679%




Sum of corrected areas: 47347491

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102820\
Data File : BP003767.D
Acq On : 28 Oct 2020 13:09
Operator : CG/JU
Sample : PB132669BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132669BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

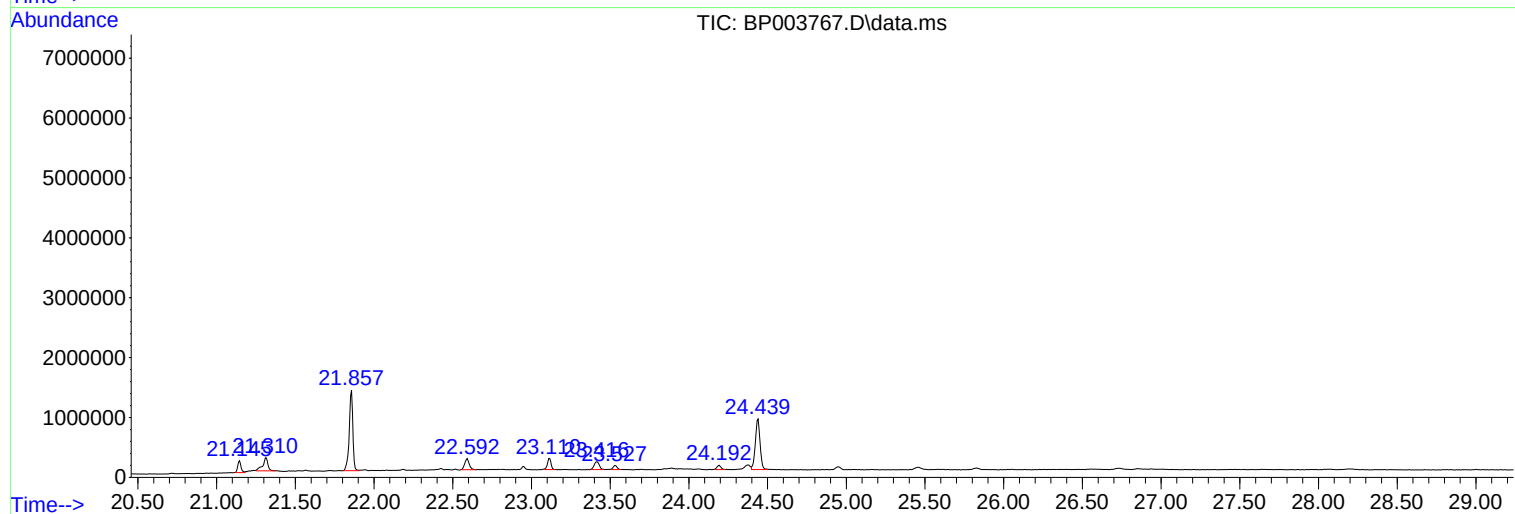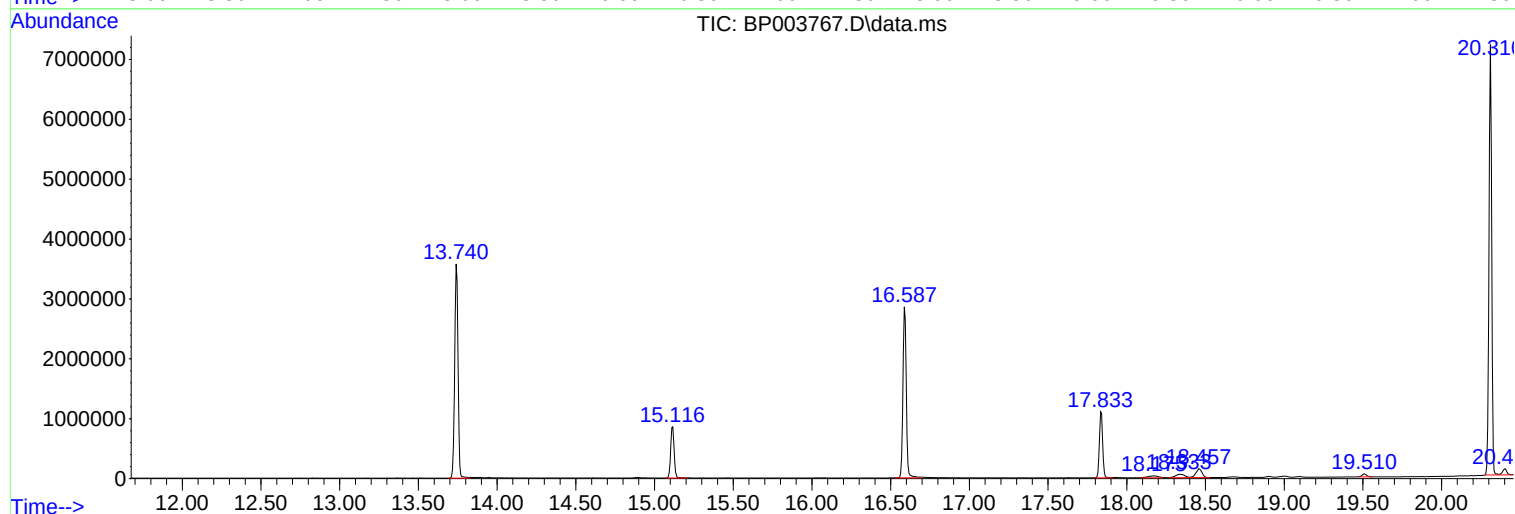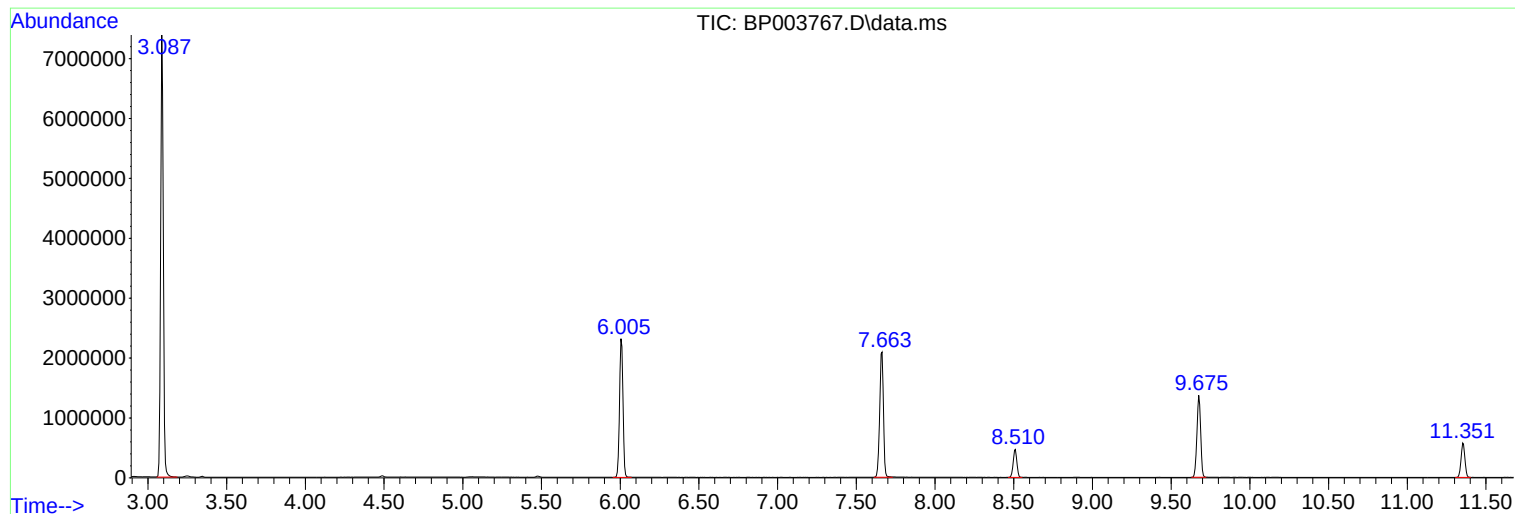

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102820\
Data File : BP003767.D
Acq On : 28 Oct 2020 13:09
Operator : CG/JU
Sample : PB132669BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132669BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102820\
Data File : BP003767.D
Acq On : 28 Oct 2020 13:09
Operator : CG/JU
Sample : PB132669BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132669BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------