
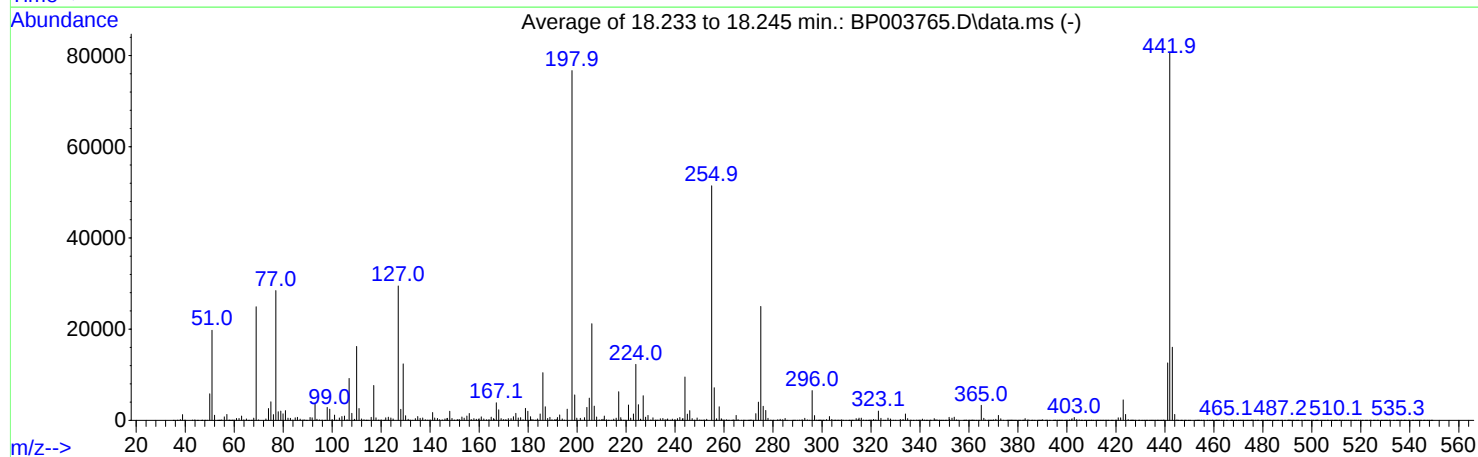


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102820\
Data File : BP003765.D
Acq On : 28 Oct 2020 09:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 26 16:22:21 2020

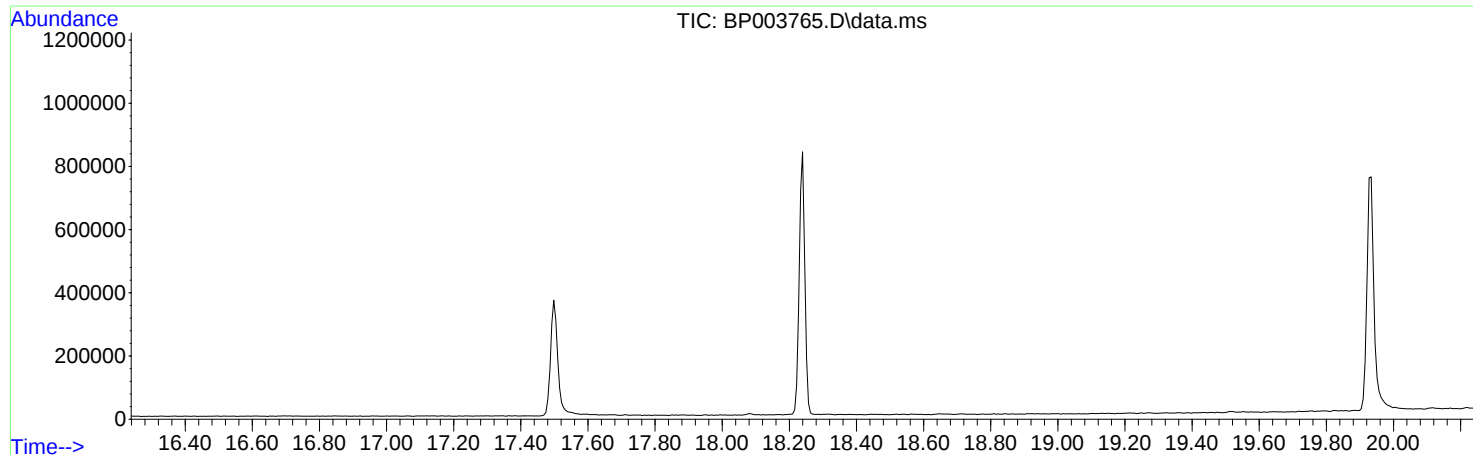

AutoFind: Scans 2609, 2610, 2611; Background Corrected with Scan 2601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	19750	PASS
68	69	0.00	2	2.0	496	PASS
69	198	0.00	100	32.5	24915	PASS
70	69	0.00	2	0.4	93	PASS
127	198	10	80	38.4	29460	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76697	PASS
199	198	5	9	7.3	5574	PASS
275	198	10	60	32.6	24997	PASS
365	198	1	100	4.3	3293	PASS
441	198	0.01	100	16.4	12598	PASS
442	442	100	100	100.0	80677	PASS
443	442	15	24	19.9	16024	PASS