




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022692.D
Acq On : 28 Oct 2024 23:02
Operator : RC/JU
Sample : P4530-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H34

Manual IntegrationsAPPROVED

Quant Time: Oct 29 01:25:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 26 05:55:04 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/29/2024
Supervised By :mohammad ahmed 10/30/2024

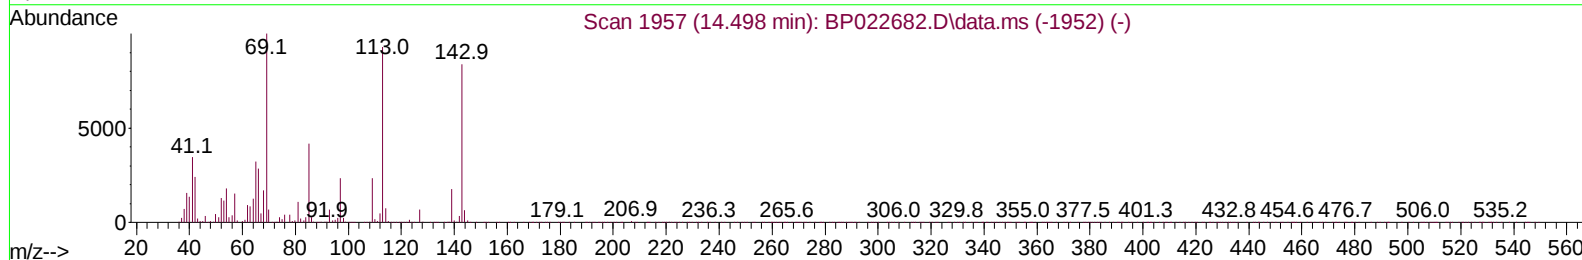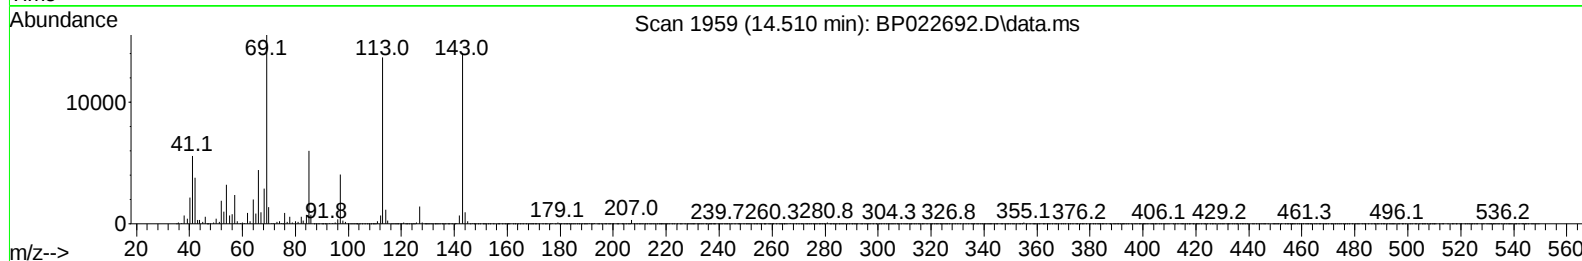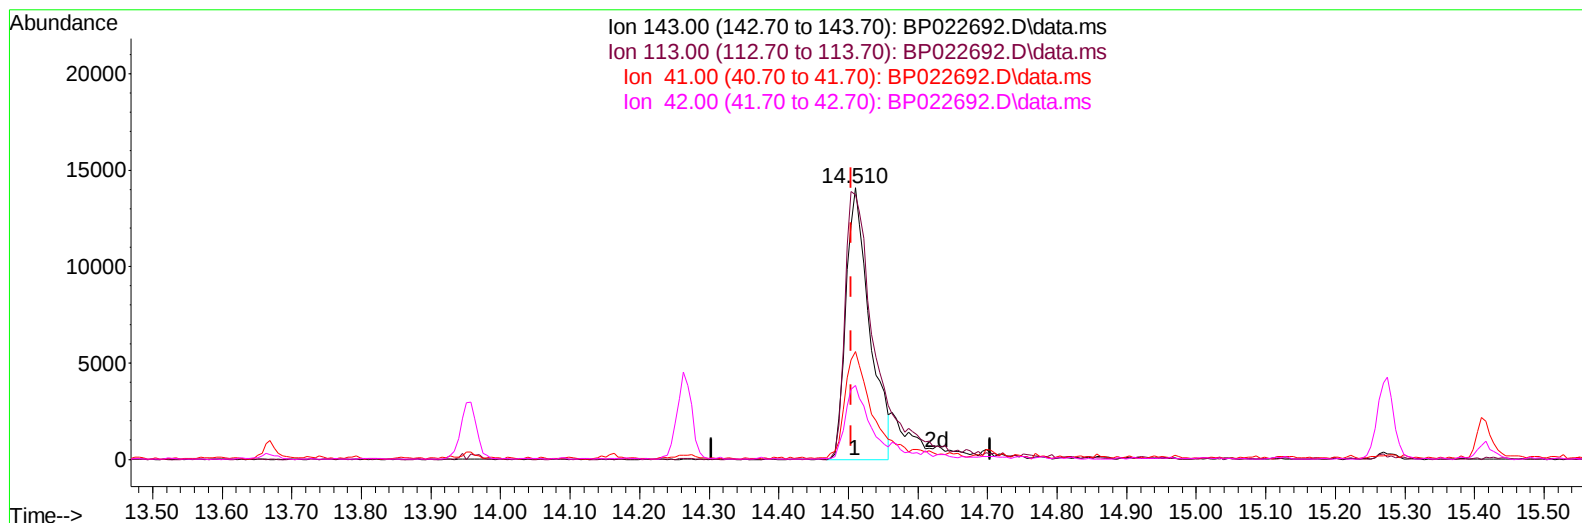

TIC: BP022692.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.510min (+ 0.006) 11.95 ng/u1

response 33062

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	97.41
41.00	35.90	39.81
42.00	23.70	27.14




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
 Data File : BP022692.D
 Acq On : 28 Oct 2024 23:02
 Operator : RC/JU
 Sample : P4530-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7H34

Manual IntegrationsAPPROVED

Quant Time: Oct 29 01:25:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 26 05:55:04 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/29/2024
 Supervised By :mohammad ahmed 10/30/2024

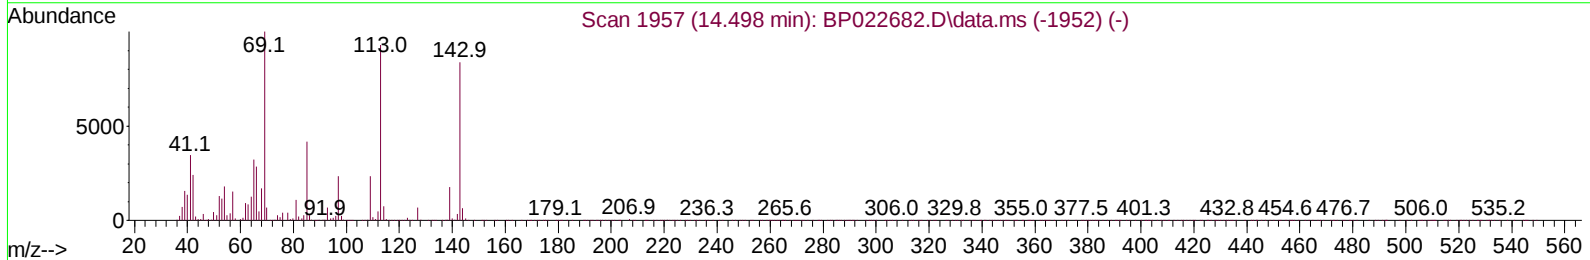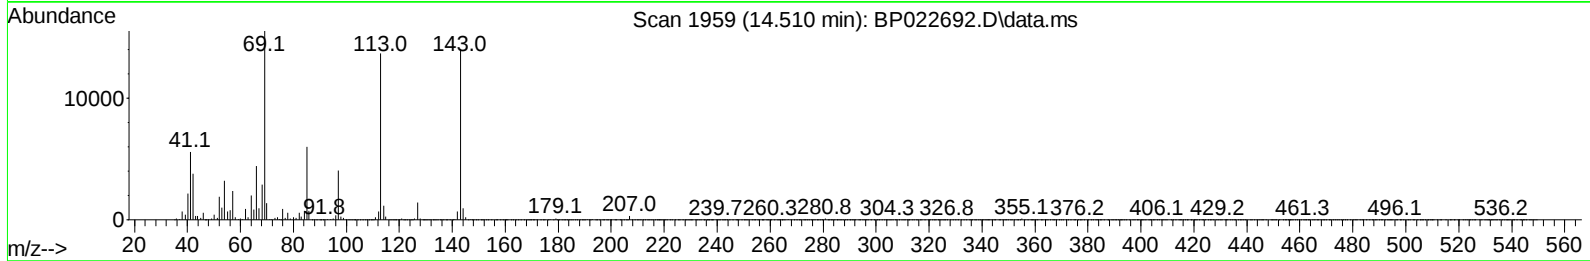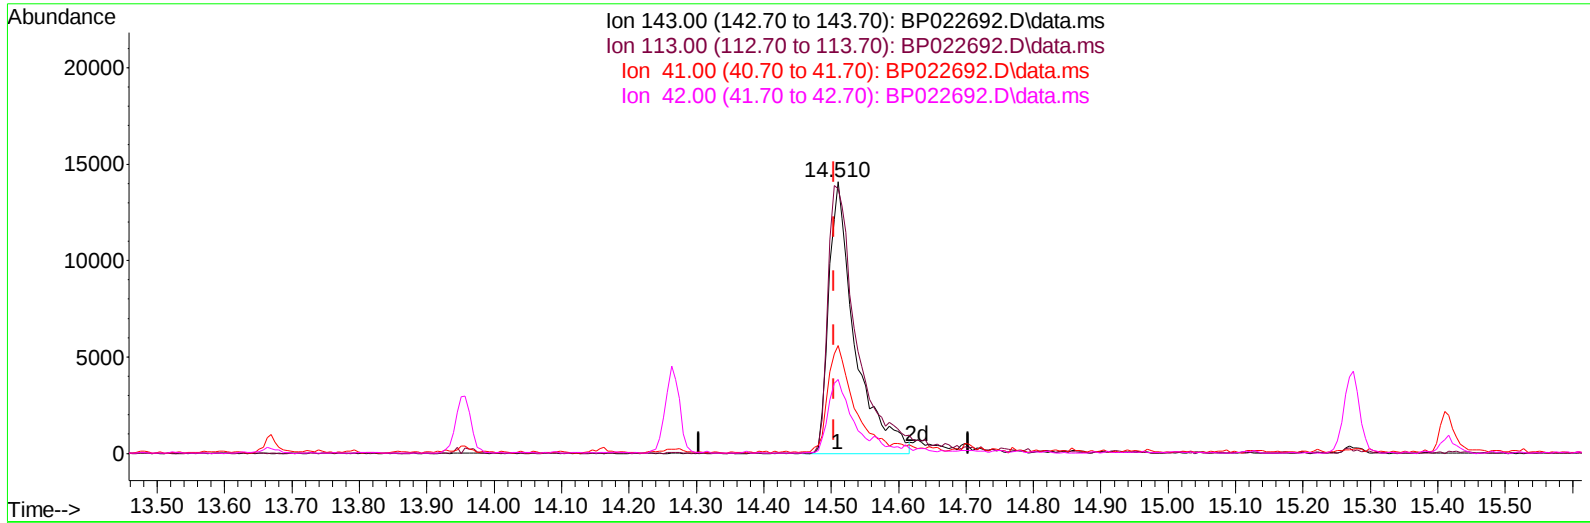

TIC: BP022692.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.510min (+ 0.006) 13.63 ng/ul m

response 37708

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	97.41
41.00	35.90	39.81
42.00	23.70	27.14

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
 Data File : BP022692.D
 Acq On : 28 Oct 2024 23:02
 Operator : RC/JU
 Sample : P4530-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7H34

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/29/2024
 Supervised By :mohammad ahmed 10/30/2024

Quant Time: Oct 29 01:28:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 26 05:55:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	75806	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.404	136	275505	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.263	164	207613	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.069	188	521367	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.492	240	608415	20.000	ng/ul	0.00
88) Perylene-d12	24.745	264	762706	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	6899	3.537	ng/uL	-0.01
4) Pyridine-d5	3.599	84	86250	16.106	ng/ul	-0.01
7) Phenol-d5	6.840	99	113117	17.727	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	6.993	67	65462	17.454	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.187	132	84048	18.562	ng/ul	-0.02
15) 4-Methylphenol-d8	8.352	113	91759	18.019	ng/ul	-0.01
21) Nitrobenzene-d5	8.793	128	41541	19.610	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	48114	19.618	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	93710	17.978	ng/ul	0.00
31) 4-Chloroaniline-d4	10.551	131	106940	17.363	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	352507	21.370	ng/ul	-0.01
49) Acenaphthylene-d8	13.957	160	358930	20.487	ng/ul	0.00
54) 4-Nitrophenol-d4	14.510	143	37708m	13.626	ng/ul	0.00
60) Fluorene-d10	15.269	176	307867	21.518	ng/ul	-0.02
65) 4,6-Dinitro-2-methylph...	15.416	200	46507	13.563	ng/ul	0.00
73) Anthracene-d10	17.169	188	521367	21.257	ng/ul	0.00
81) Pyrene-d10	19.551	212	668342	20.773	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.533	264	867965	21.309	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022692.D
Acq On : 28 Oct 2024 23:02
Operator : RC/JU
Sample : P4530-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H34

Manual IntegrationsAPPROVED

Quant Time: Oct 29 01:28:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 26 05:55:04 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/29/2024
Supervised By :mohammad ahmed 10/30/2024

