




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
 Data File : BP022704.D
 Acq On : 29 Oct 2024 07:45
 Operator : RC/JU
 Sample : P4530-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7H41

Manual IntegrationsAPPROVED

Quant Time: Oct 29 08:11:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 29 04:53:07 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/30/2024
 Supervised By :mohammad ahmed 10/30/2024

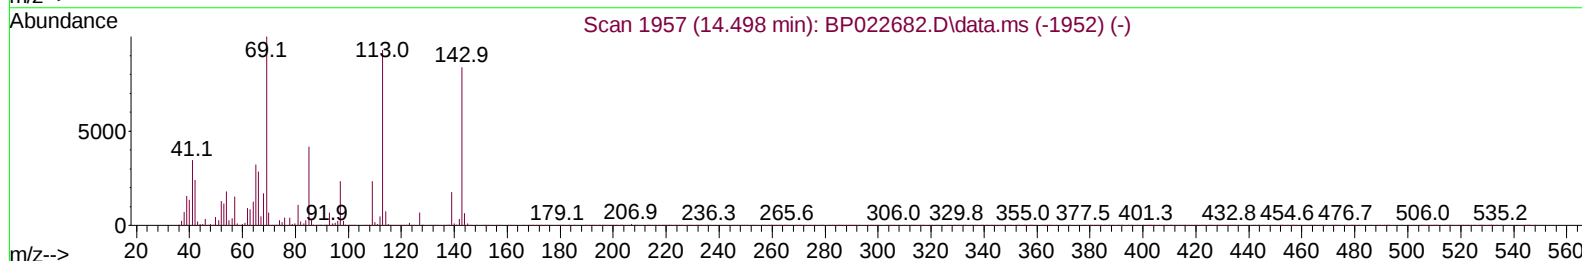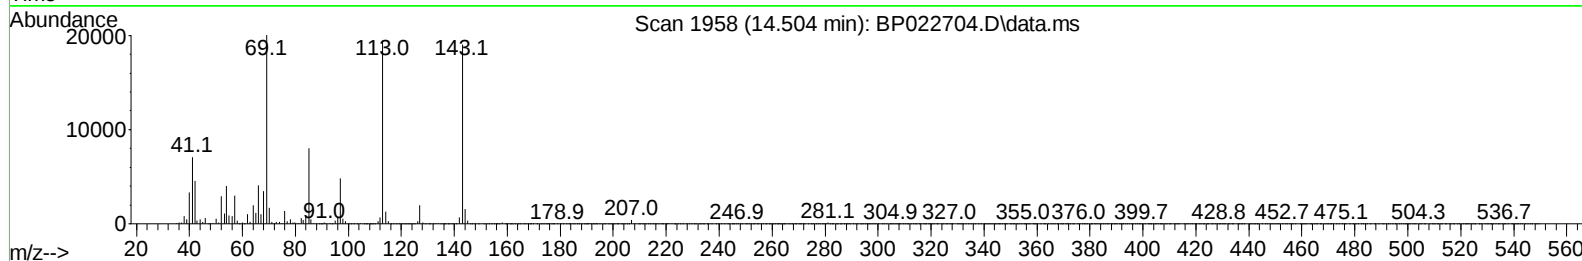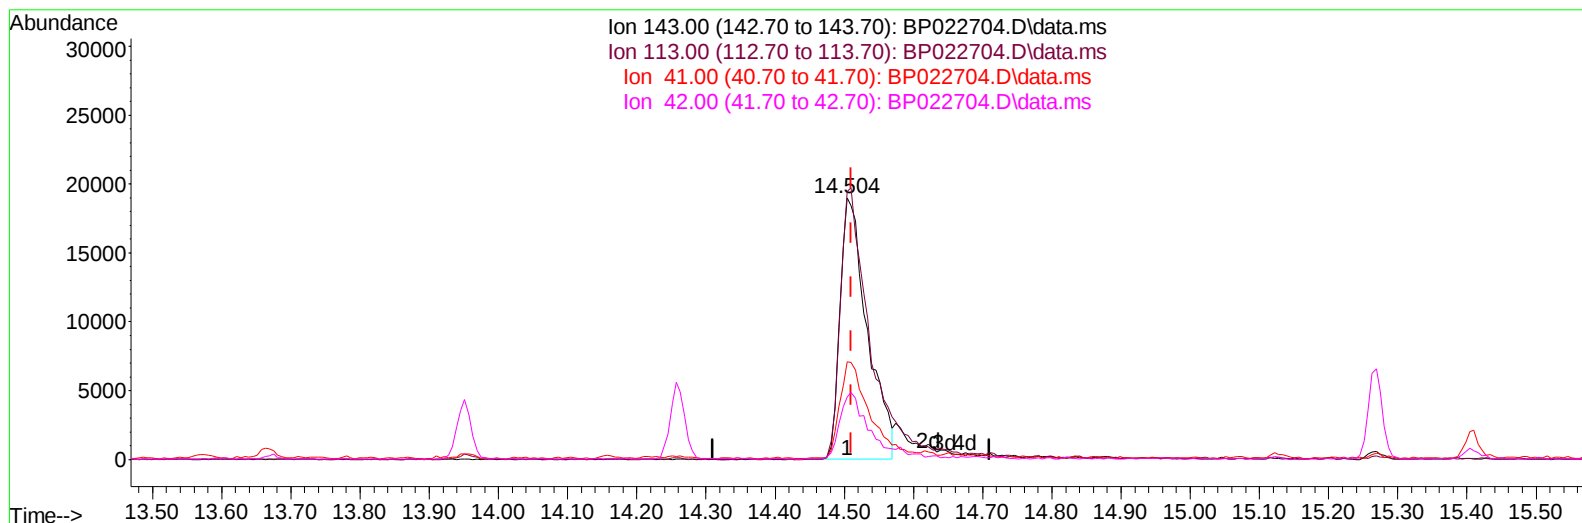

TIC: BP022704.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.504min (-0.006) 14.16 ng/u1

response 51765

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	102.31
41.00	35.90	37.29
42.00	23.70	23.91




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022704.D
Acq On : 29 Oct 2024 07:45
Operator : RC/JU
Sample : P4530-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H41

Manual IntegrationsAPPROVED

Quant Time: Oct 29 08:11:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 29 04:53:07 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/30/2024
Supervised By :mohammad ahmed 10/30/2024

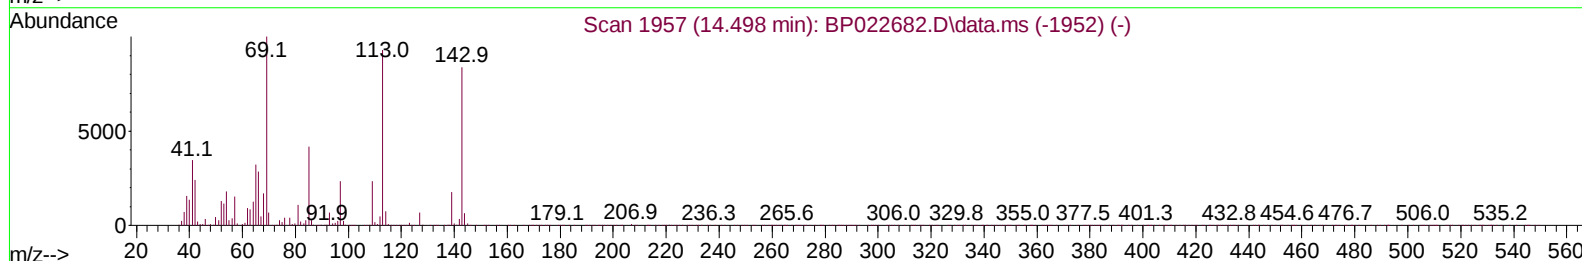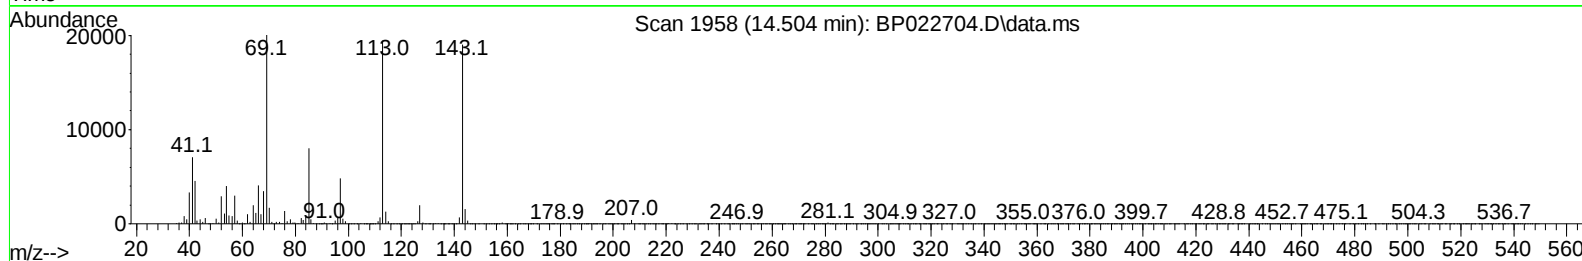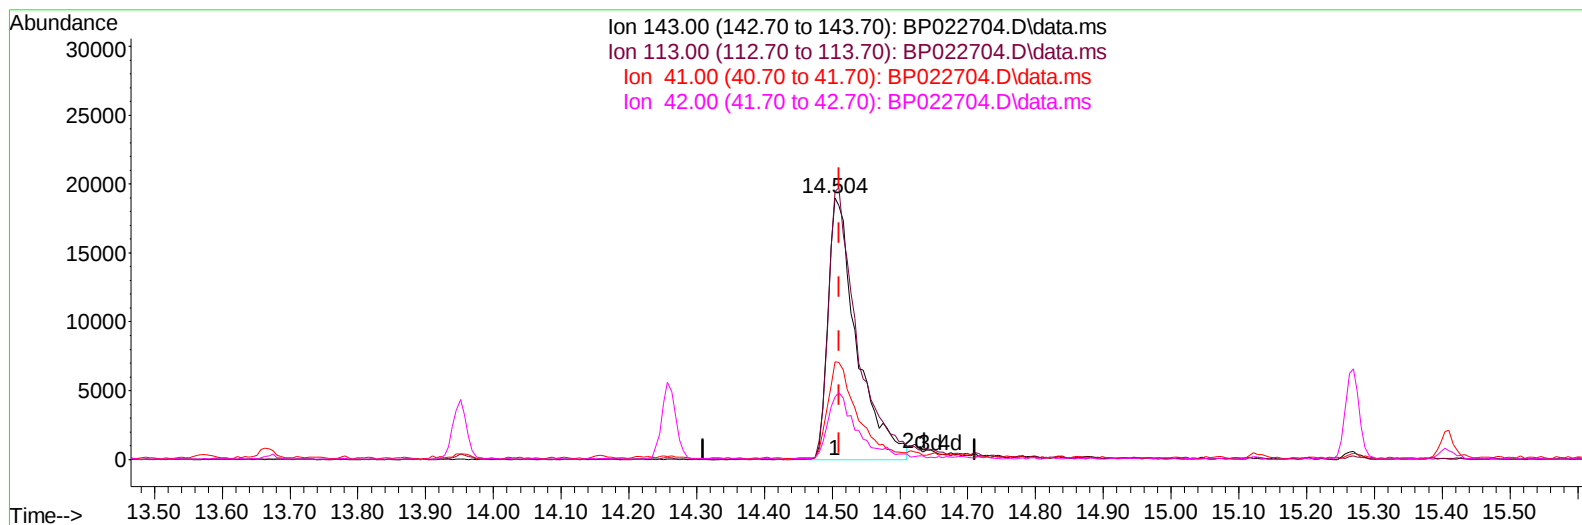

TIC: BP022704.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.504min (-0.006) 15.28 ng/ul m

response 55836

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	102.31
41.00	35.90	37.29
42.00	23.70	23.91

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
 Data File : BP022704.D
 Acq On : 29 Oct 2024 07:45
 Operator : RC/JU
 Sample : P4530-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7H41

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/30/2024
 Supervised By :mohammad ahmed 10/30/2024

Quant Time: Oct 29 08:13:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 29 04:53:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	89312	20.000	ng/ul	0.00
20) Naphthalene-d8	10.398	136	340369	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.257	164	274230	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	677287	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	720589	20.000	ng/ul	0.00
88) Perylene-d12	24.757	264	855493	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	6804	2.960	ng/uL	0.00
4) Pyridine-d5	3.605	84	41100	6.514	ng/ul	0.01
7) Phenol-d5	6.840	99	145388	19.339	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	84704	19.170	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	106626	19.988	ng/ul	0.00
15) 4-Methylphenol-d8	8.352	113	121729	20.289	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	54650	20.882	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	66590	21.977	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	131319	20.392	ng/ul	0.00
31) 4-Chloroaniline-d4	10.546	131	125614	16.508	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	471879	21.658	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	507955	21.950	ng/ul	0.00
54) 4-Nitrophenol-d4	14.504	143	55836m	15.276	ng/ul	0.00
60) Fluorene-d10	15.269	176	429199	22.711	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.410	200	51799	11.629	ng/ul	0.00
73) Anthracene-d10	17.157	188	732674	22.996	ng/ul	0.00
81) Pyrene-d10	19.533	212	909188	23.859	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.521	264	1066520	23.344	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022704.D
Acq On : 29 Oct 2024 07:45
Operator : RC/JU
Sample : P4530-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H41

Manual IntegrationsAPPROVED

Quant Time: Oct 29 08:13:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 29 04:53:07 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/30/2024
Supervised By :mohammad ahmed 10/30/2024

