

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
 Data File : BP022699.D
 Acq On : 29 Oct 2024 04:24
 Operator : RC/JU
 Sample : PB164432BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK432

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	30	33	40	rBV	18895	27657	1.25%	0.133%
2	3.599	100	104	125	rBV	219438	357480	16.20%	1.725%
3	3.910	154	157	164	rVB2	4173	6251	0.28%	0.030%
4	6.793	642	647	649	rBV5	2907	4405	0.20%	0.021%
5	6.840	649	655	666	rVV	250859	426515	19.33%	2.058%
6	6.993	674	681	690	rVB	198896	312834	14.18%	1.510%
7	7.193	708	715	728	rBV	267181	436672	19.79%	2.107%
8	7.645	784	792	801	rBV	281219	447922	20.30%	2.162%
9	8.351	906	912	921	rBV	300392	532282	24.13%	2.569%
10	8.534	941	943	947	rBV4	1569	2361	0.11%	0.011%
11	8.792	976	987	997	rBV	252576	438929	19.89%	2.118%
12	9.192	1049	1055	1059	rBV6	3548	6136	0.28%	0.030%
13	9.504	1101	1108	1118	rBV	227063	376610	17.07%	1.817%
14	10.045	1193	1200	1216	rBV	302290	577175	26.16%	2.785%
15	10.145	1216	1217	1225	rVB8	4183	6056	0.27%	0.029%
16	10.404	1253	1261	1270	rBV	345191	598789	27.14%	2.890%
17	10.545	1276	1285	1301	rBV	277488	549096	24.89%	2.650%
18	10.692	1308	1310	1319	rVB9	1529	3115	0.14%	0.015%
19	11.669	1472	1476	1483	rVB6	2990	5767	0.26%	0.028%
20	12.004	1528	1533	1534	rBV3	3968	4735	0.21%	0.023%
21	13.669	1810	1816	1829	rBV	632913	975416	44.21%	4.707%
22	13.951	1855	1864	1885	rBV2	713095	1068445	48.43%	5.156%
23	14.263	1910	1917	1926	rBV	705503	944641	42.82%	4.559%
24	14.510	1951	1959	1983	rBV2	142517	441647	20.02%	2.131%
25	15.274	2081	2089	2099	rBV	919061	1419316	64.33%	6.849%
26	15.410	2106	2112	2125	rBV	298046	443075	20.08%	2.138%
27	15.510	2126	2129	2134	rVB6	5074	8637	0.39%	0.042%
28	16.833	2351	2354	2359	rBV5	2082	3630	0.16%	0.018%
29	17.063	2387	2393	2402	rBV	952265	1269541	57.54%	6.126%
30	17.157	2403	2409	2423	rVV	1114978	1631083	73.93%	7.871%
31	17.363	2440	2444	2445	rBV4	1919	2387	0.11%	0.012%
32	18.004	2549	2553	2558	rVV6	5301	10105	0.46%	0.049%
33	19.092	2734	2738	2742	rBV3	13791	20456	0.93%	0.099%
34	19.162	2747	2750	2755	rVV2	12215	18429	0.84%	0.089%
35	19.539	2809	2814	2830	rBV	1412420	2024129	91.75%	9.768%
36	21.486	3138	3145	3155	rBV	890920	1538173	69.72%	7.423%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022699.D
Acq On : 29 Oct 2024 04:24
Operator : RC/JU
Sample : PB164432BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK432

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.527	3651	3662	3674	rVB2	780009	2206238	100.00%	10.647%
38	24.739	3690	3698	3712	rVB	587839	1576059	71.44%	7.606%




Sum of corrected areas: 20722194

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022699.D
Acq On : 29 Oct 2024 04:24
Operator : RC/JU
Sample : PB164432BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK432

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

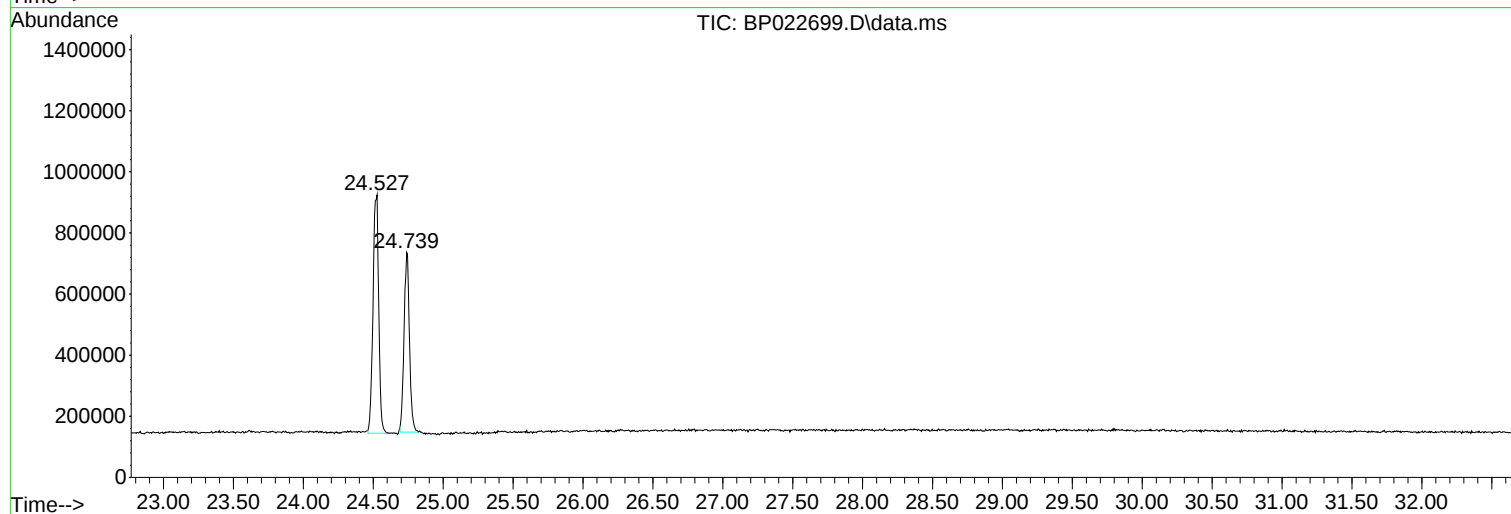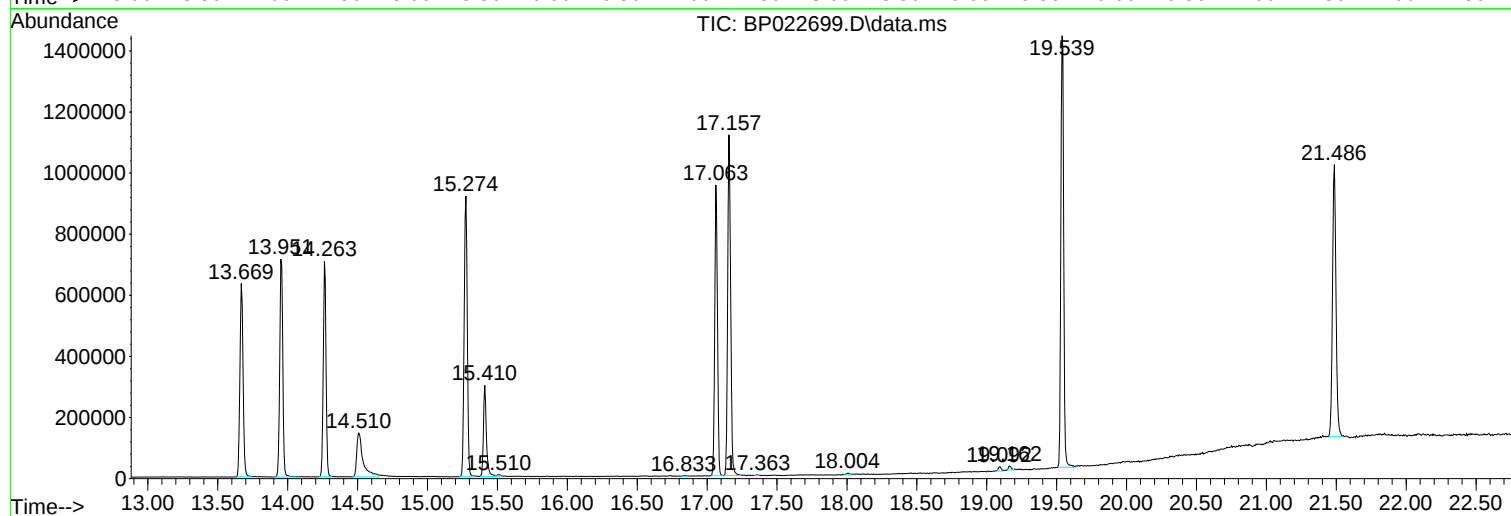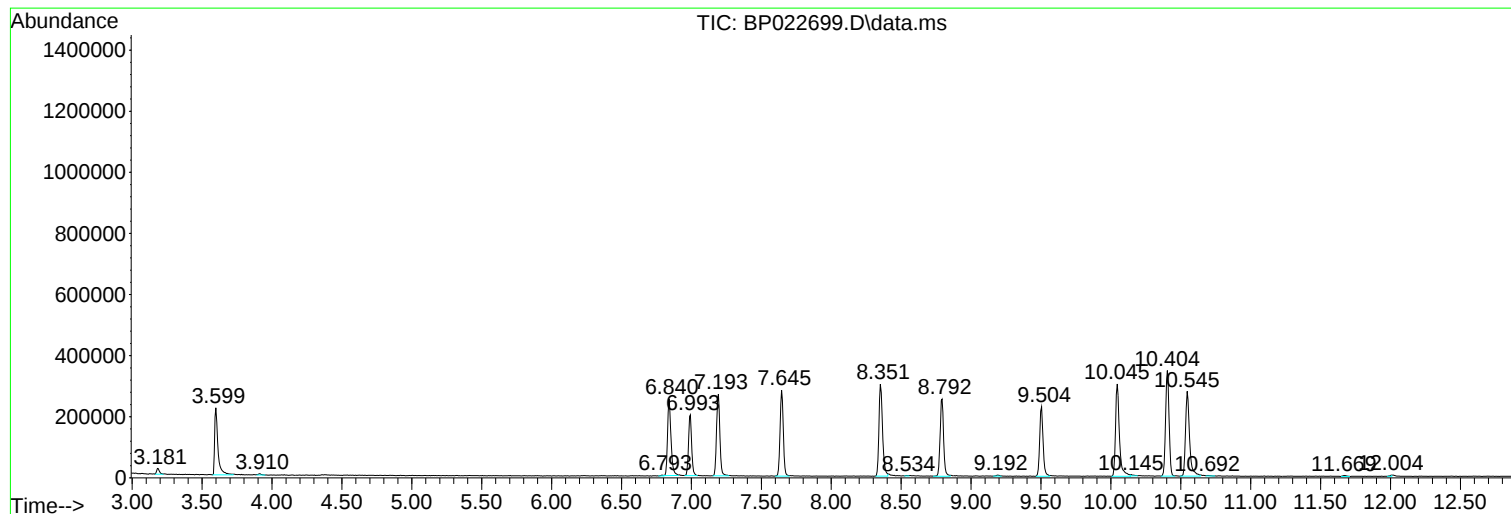

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022699.D
Acq On : 29 Oct 2024 04:24
Operator : RC/JU
Sample : PB164432BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK432

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022699.D
Acq On : 29 Oct 2024 04:24
Operator : RC/JU
Sample : PB164432BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK432

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc