

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
 Data File : BP022710.D
 Acq On : 29 Oct 2024 11:48
 Operator : RC/JU
 Sample : PB164416BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK416

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	40	rVB	19510	23137	1.05%	0.114%
2	3.593	99	103	115	rBV	218507	334167	15.16%	1.639%
3	3.911	153	157	162	rVB3	4454	7299	0.33%	0.036%
4	6.787	641	646	649	rBV3	2852	4606	0.21%	0.023%
5	6.834	649	654	671	rVV	254411	439096	19.92%	2.154%
6	6.987	673	680	693	rVV	201184	310349	14.08%	1.523%
7	7.187	707	714	727	rBV	273956	437072	19.83%	2.144%
8	7.640	783	791	801	rBV	257176	413744	18.77%	2.030%
9	8.346	903	911	931	rBV	287359	554542	25.16%	2.721%
10	8.787	978	986	995	rBV	242409	430044	19.51%	2.110%
11	9.181	1049	1053	1059	rVB6	4297	7020	0.32%	0.034%
12	9.493	1099	1106	1117	rBV	200881	374886	17.01%	1.839%
13	10.040	1191	1199	1221	rBV	309362	598917	27.18%	2.938%
14	10.399	1251	1260	1269	rBV	357756	567421	25.75%	2.784%
15	10.540	1275	1284	1307	rBV	273204	553860	25.13%	2.717%
16	11.669	1471	1476	1481	rVB6	4391	6118	0.28%	0.030%
17	12.004	1526	1533	1542	rBV6	4216	9795	0.44%	0.048%
18	13.675	1809	1817	1827	rBV	646361	951490	43.17%	4.668%
19	13.951	1856	1864	1878	rBV2	663202	1060037	48.10%	5.201%
20	14.257	1909	1916	1925	rBV	583816	892005	40.47%	4.376%
21	14.498	1951	1957	1975	rBV	138050	420094	19.06%	2.061%
22	15.269	2079	2088	2096	rBV	928854	1410577	64.00%	6.921%
23	15.422	2108	2114	2124	rVV	271798	390079	17.70%	1.914%
24	15.516	2127	2130	2137	rVB5	8199	13217	0.60%	0.065%
25	16.539	2299	2304	2310	rBV10	2323	4726	0.21%	0.023%
26	16.739	2332	2338	2340	rBV7	2316	3507	0.16%	0.017%
27	16.845	2354	2356	2362	rVB6	2935	3627	0.16%	0.018%
28	17.063	2386	2393	2402	rBV	791201	1208259	54.82%	5.928%
29	17.169	2404	2411	2426	rVB	1175023	1654894	75.09%	8.119%
30	18.022	2550	2556	2559	rBV7	2840	5243	0.24%	0.026%
31	18.586	2651	2652	2655	rBV3	2662	2918	0.13%	0.014%
32	19.092	2733	2738	2742	rVB4	11733	18217	0.83%	0.089%
33	19.157	2746	2749	2754	rVB2	12622	18648	0.85%	0.091%
34	19.539	2808	2814	2824	rBV2	1363329	2063533	93.63%	10.124%
35	21.492	3140	3146	3158	rVB2	903149	1490698	67.64%	7.314%
36	24.510	3650	3659	3672	rVB	790017	2203919	100.00%	10.813%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022710.D
Acq On : 29 Oct 2024 11:48
Operator : RC/JU
Sample : PB164416BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK416

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.739	3690	3698	3709	rVB	548471	1494664	67.82%	7.333%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 20382425

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022710.D
Acq On : 29 Oct 2024 11:48
Operator : RC/JU
Sample : PB164416BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK416

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

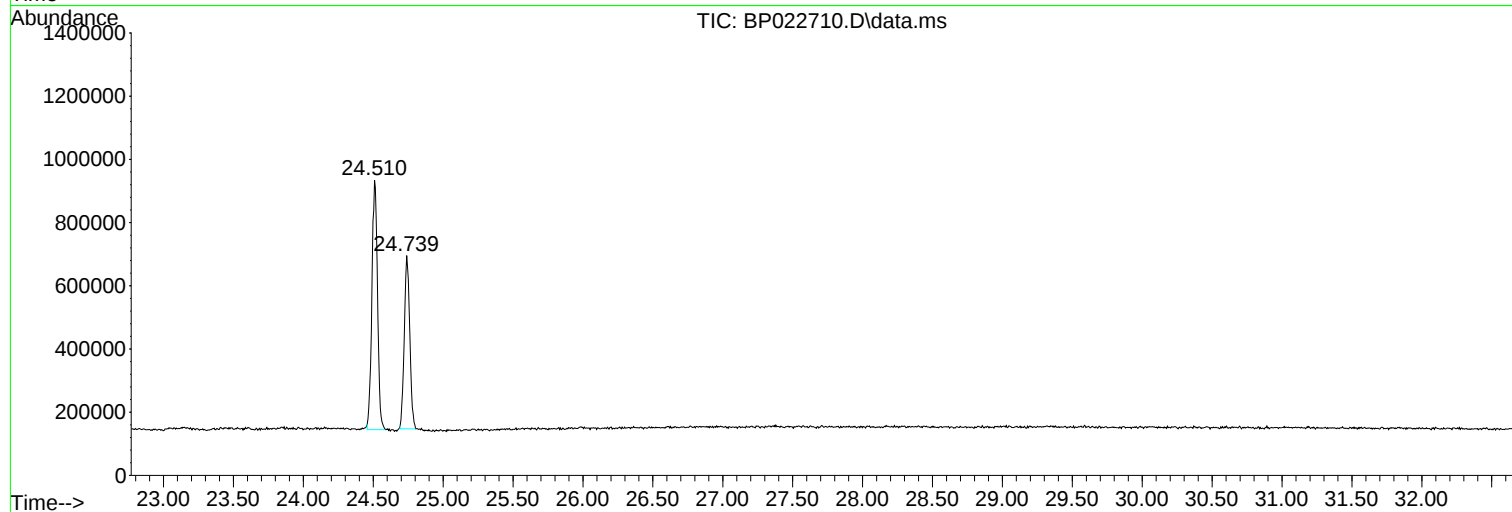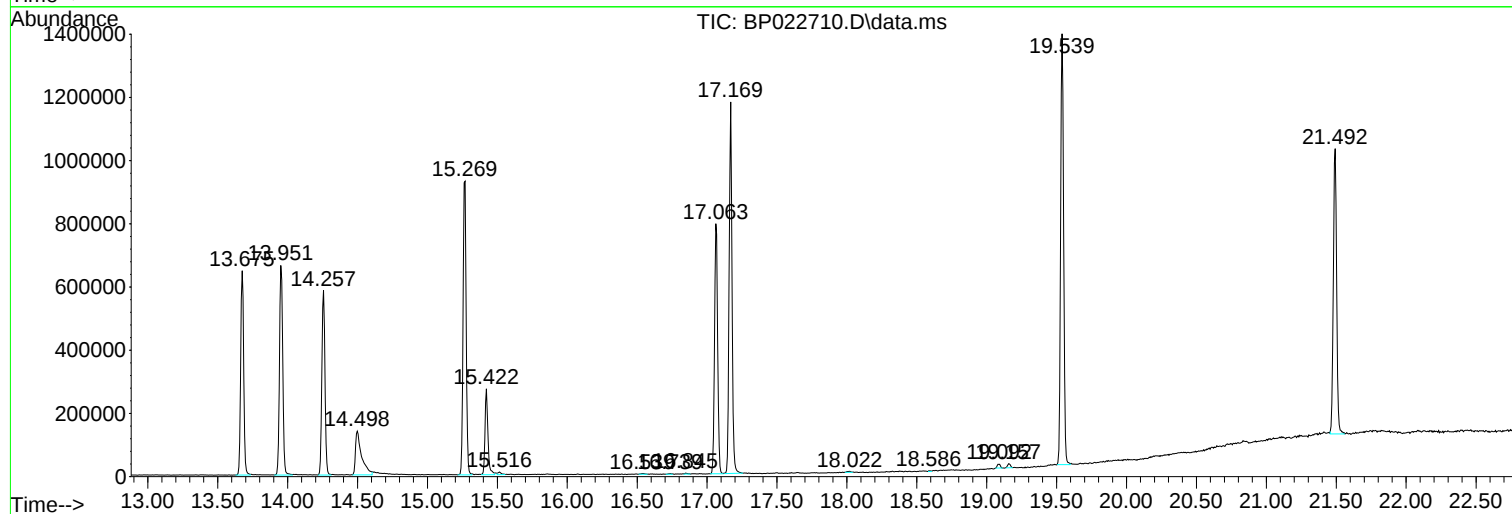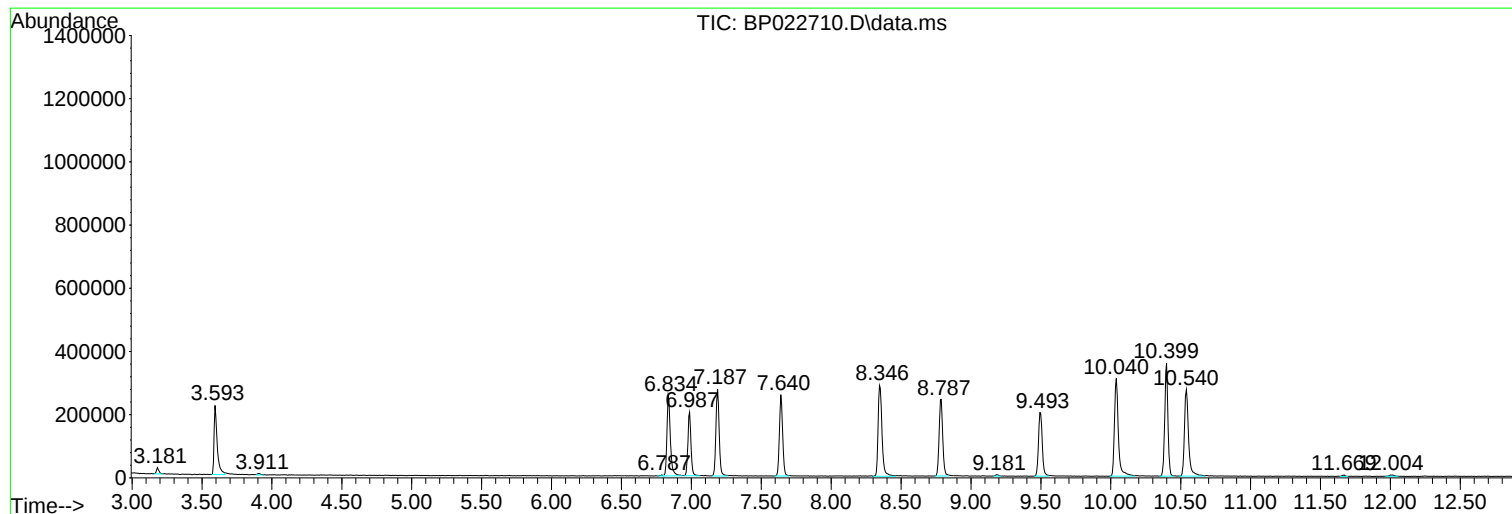

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022710.D
Acq On : 29 Oct 2024 11:48
Operator : RC/JU
Sample : PB164416BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK416

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102824\
Data File : BP022710.D
Acq On : 29 Oct 2024 11:48
Operator : RC/JU
Sample : PB164416BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK416

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc