




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022737.D
Acq On : 30 Oct 2024 15:46
Operator : RC/JU
Sample : PB164419BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK419

Manual IntegrationsAPPROVED

Quant Time: Oct 30 16:18:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

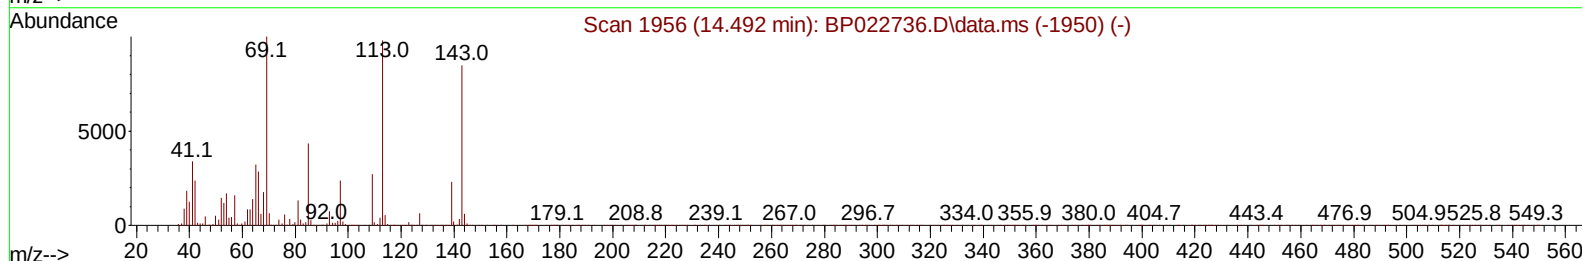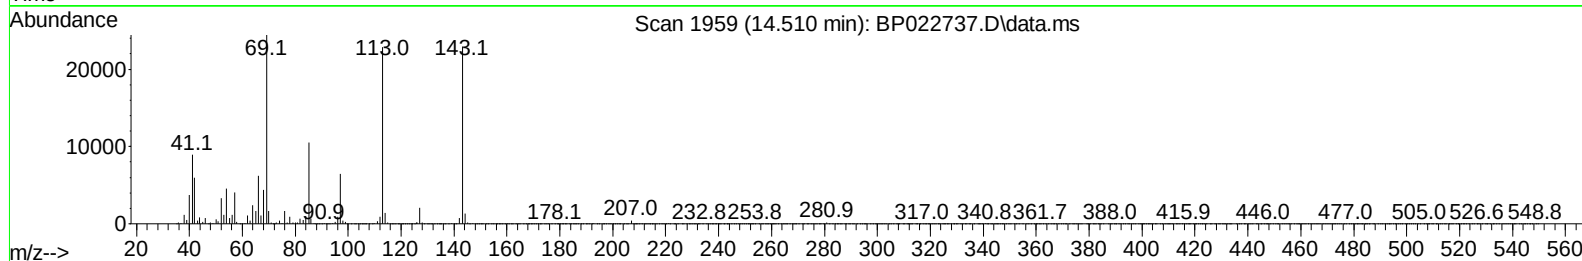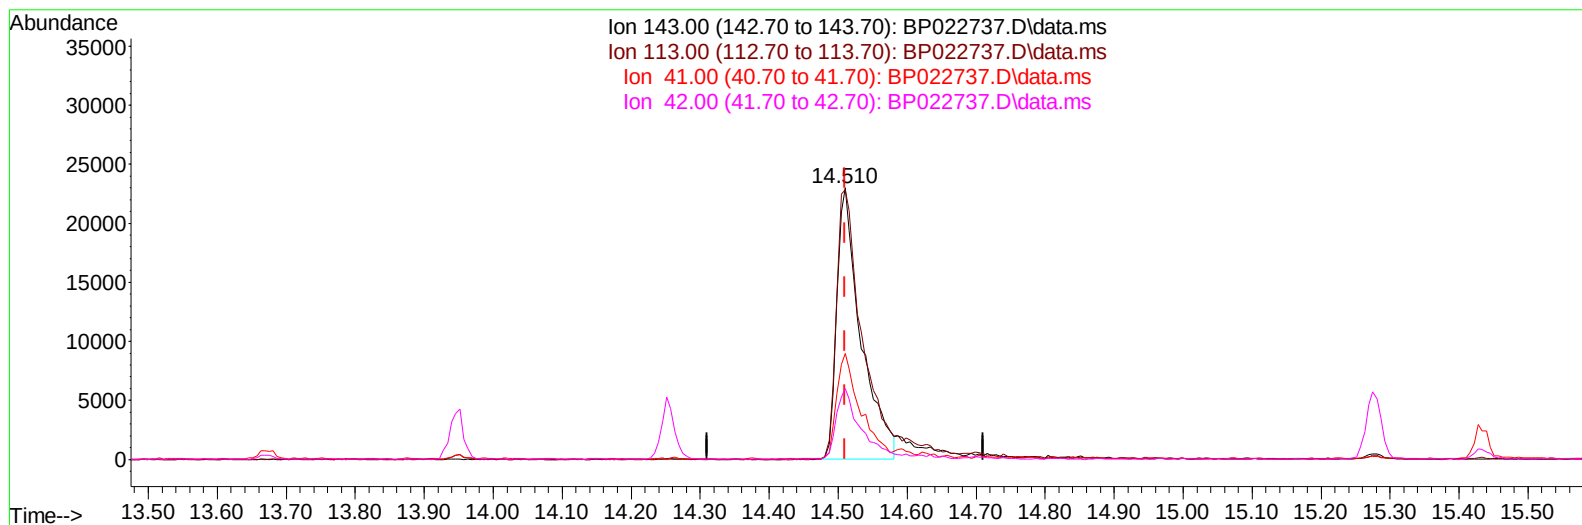

TIC: BP022737.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.510min (+ 0.000) 18.23 ng/ul

response 55465

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	99.48
41.00	35.90	38.95
42.00	23.70	25.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022737.D
Acq On : 30 Oct 2024 15:46
Operator : RC/JU
Sample : PB164419BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK419

Manual IntegrationsAPPROVED

Quant Time: Oct 30 16:18:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

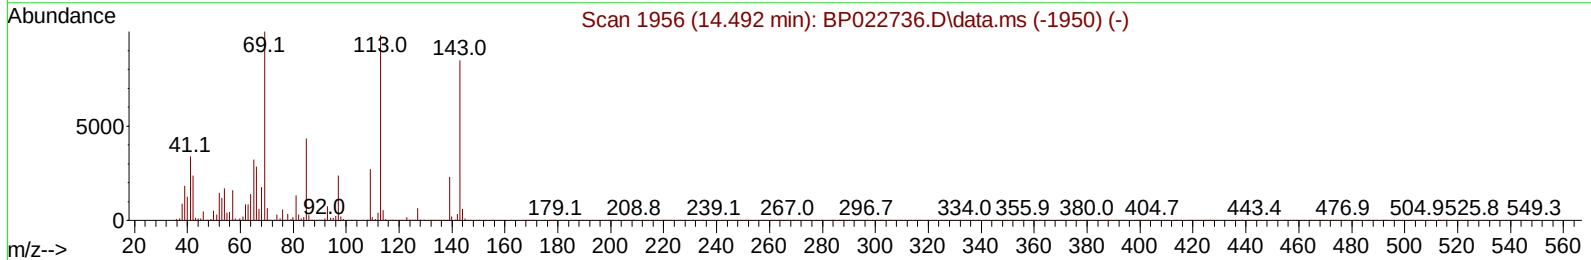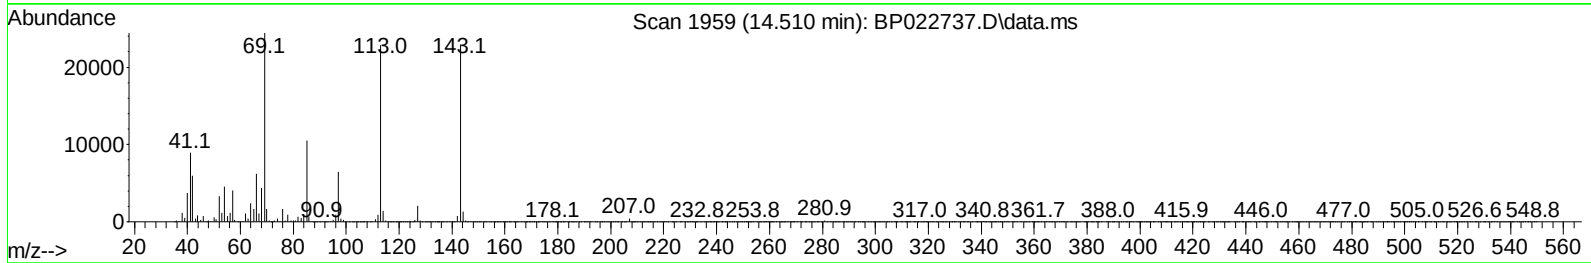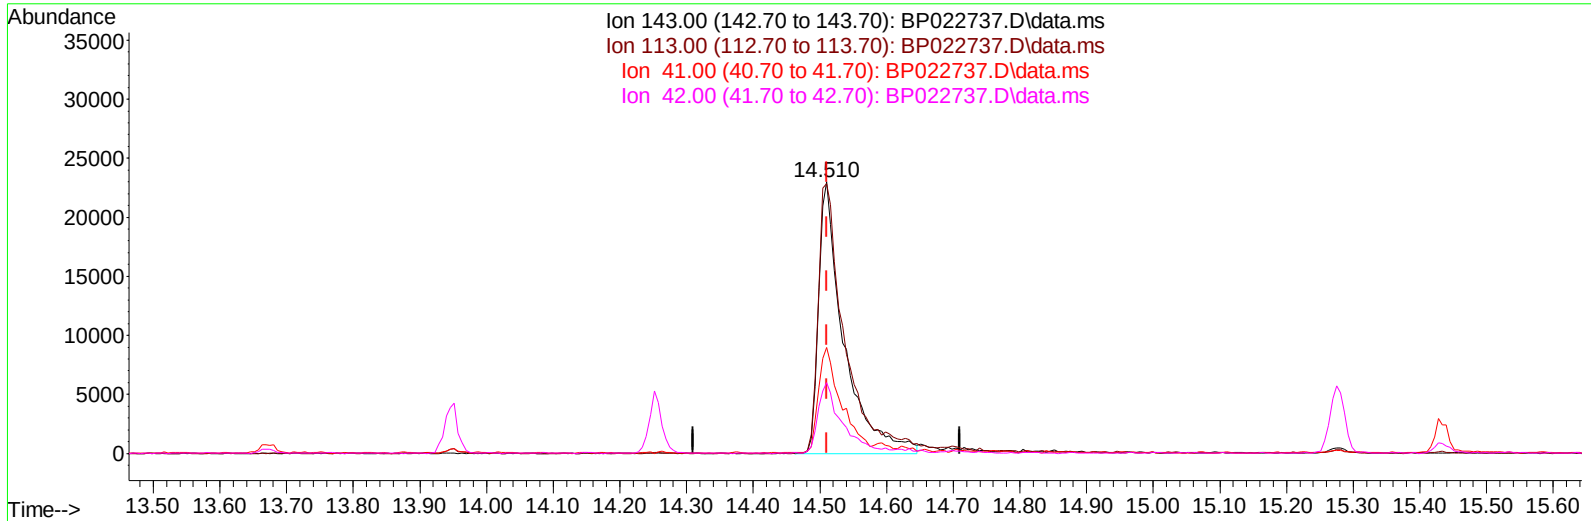

TIC: BP022737.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.510min (+ 0.000) 19.82 ng/ul m

response 60286

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	99.48
41.00	35.90	38.95
42.00	23.70	25.99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022737.D
 Acq On : 30 Oct 2024 15:46
 Operator : RC/JU
 Sample : PB164419BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK419

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Oct 30 16:23:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 30 10:56:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	73380	20.000	ng/ul	0.00
20) Naphthalene-d8	10.387	136	294287	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.257	164	228234	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.069	188	542218	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	616424	20.000	ng/ul	0.00
88) Perylene-d12	24.769	264	704832	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	8742	4.630	ng/uL	0.00
4) Pyridine-d5	3.587	84	122214	23.576	ng/ul	0.00
7) Phenol-d5	6.828	99	152005	24.609	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	87167	24.010	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	113827	25.970	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	124173	25.190	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	55312	24.444	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143	67048	25.594	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	131879	23.686	ng/ul	0.00
31) 4-Chloroaniline-d4	10.540	131	157746	23.977	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	436808	24.088	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	474598	24.642	ng/ul	0.00
54) 4-Nitrophenol-d4	14.510	143	60286m	19.817	ng/ul	0.00
60) Fluorene-d10	15.275	176	390104	24.802	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	59428	16.665	ng/ul	0.03
73) Anthracene-d10	17.175	188	651599	25.546	ng/ul	0.00
81) Pyrene-d10	19.551	212	839483	25.753	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.527	264	999834	26.562	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022737.D
Acq On : 30 Oct 2024 15:46
Operator : RC/JU
Sample : PB164419BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK419

Manual IntegrationsAPPROVED

Quant Time: Oct 30 16:23:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

