




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022761.D
Acq On : 31 Oct 2024 08:42
Operator : RC/JU
Sample : P4592-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H07

Manual IntegrationsAPPROVED

Quant Time: Oct 31 12:40:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

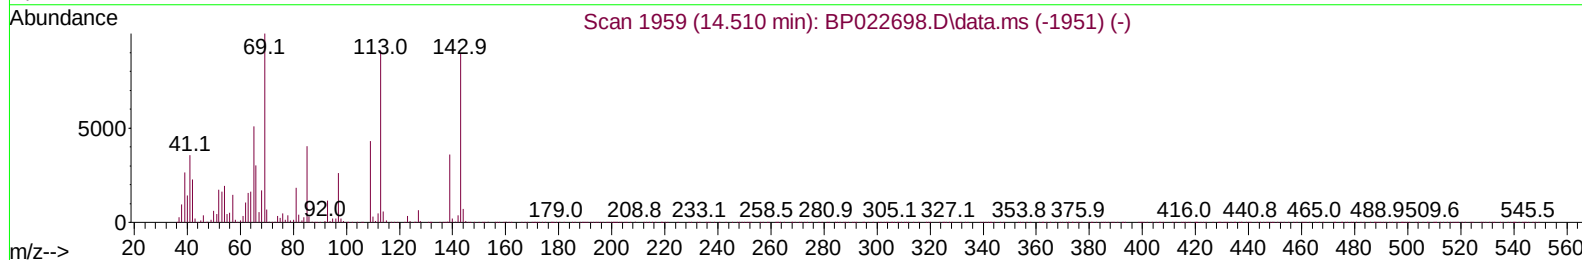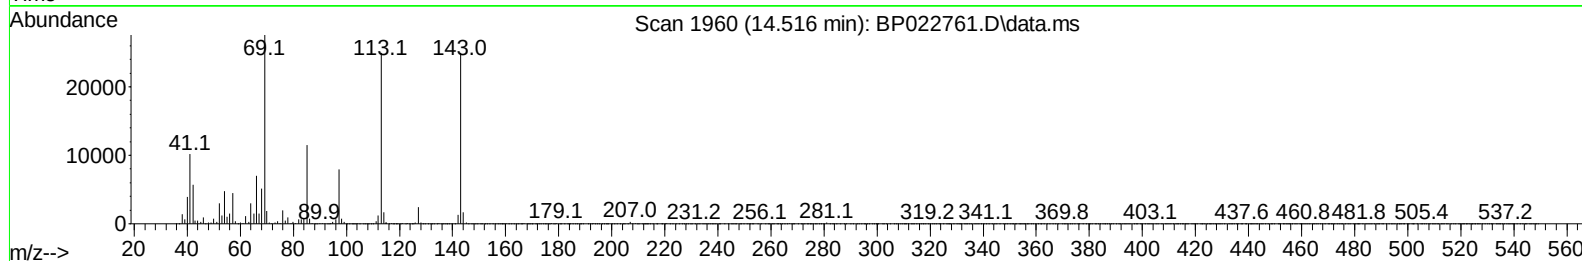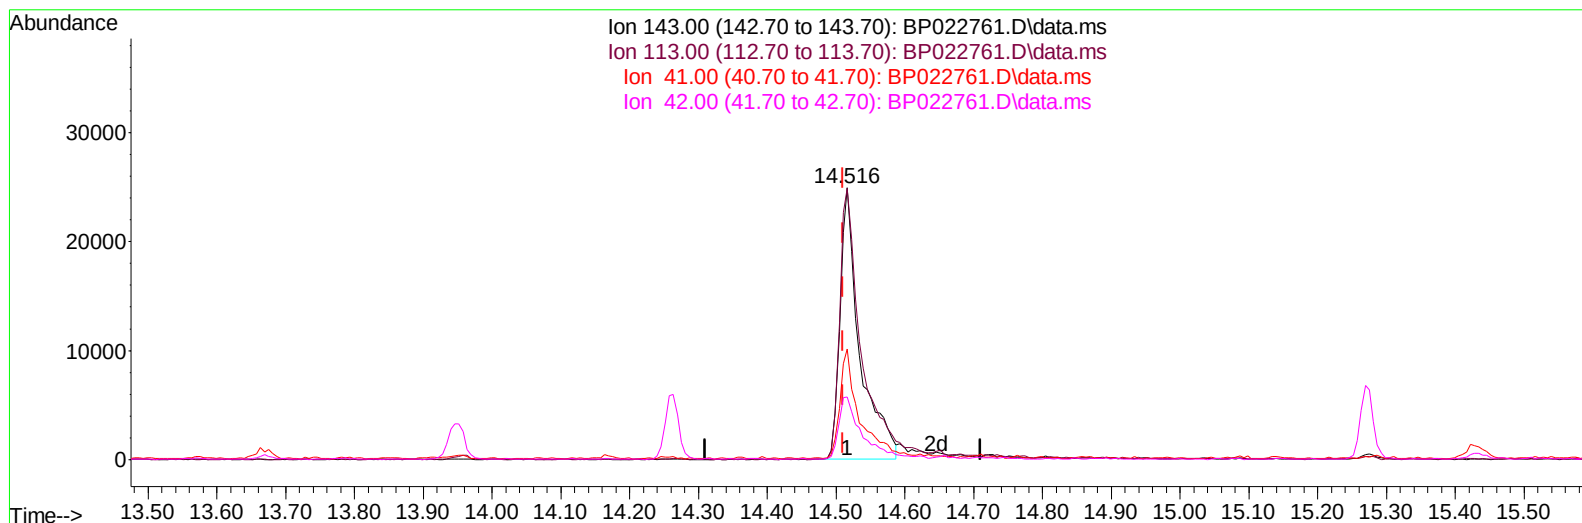

TIC: BP022761.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.516min (+ 0.006) 13.71 ng/ul

response 49922

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	99.87
41.00	35.90	40.75
42.00	23.70	22.93




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022761.D
Acq On : 31 Oct 2024 08:42
Operator : RC/JU
Sample : P4592-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H07

Manual IntegrationsAPPROVED

Quant Time: Oct 31 12:40:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

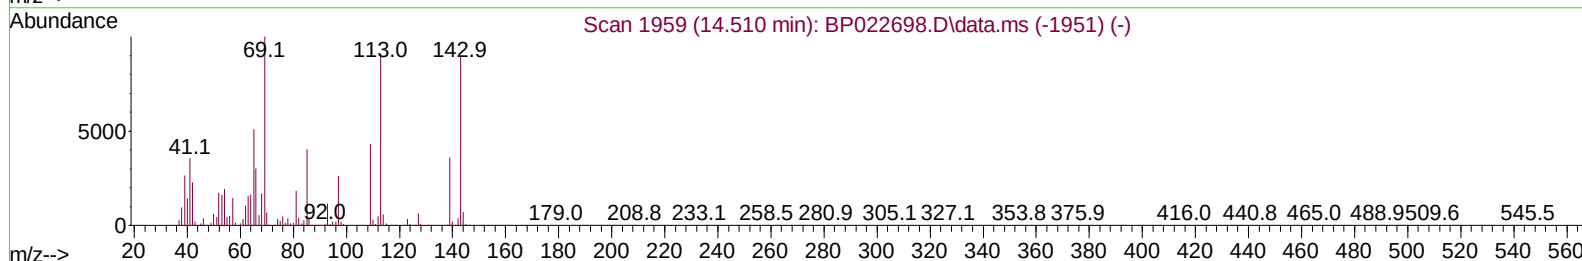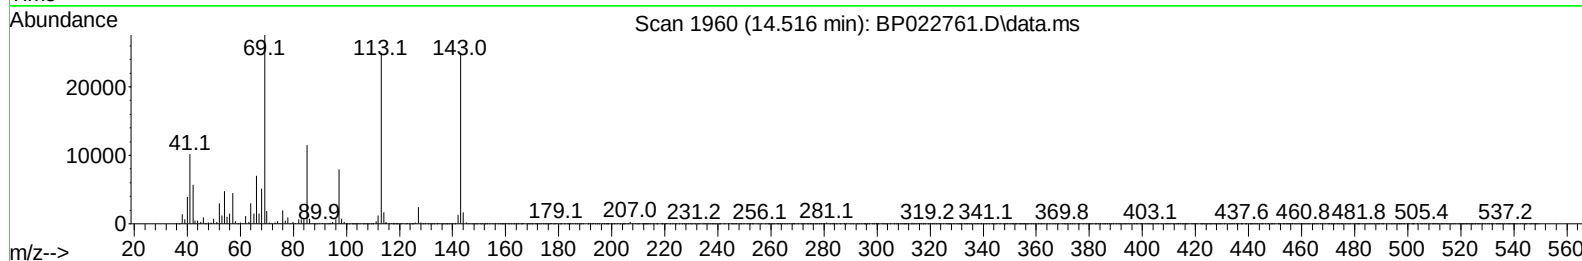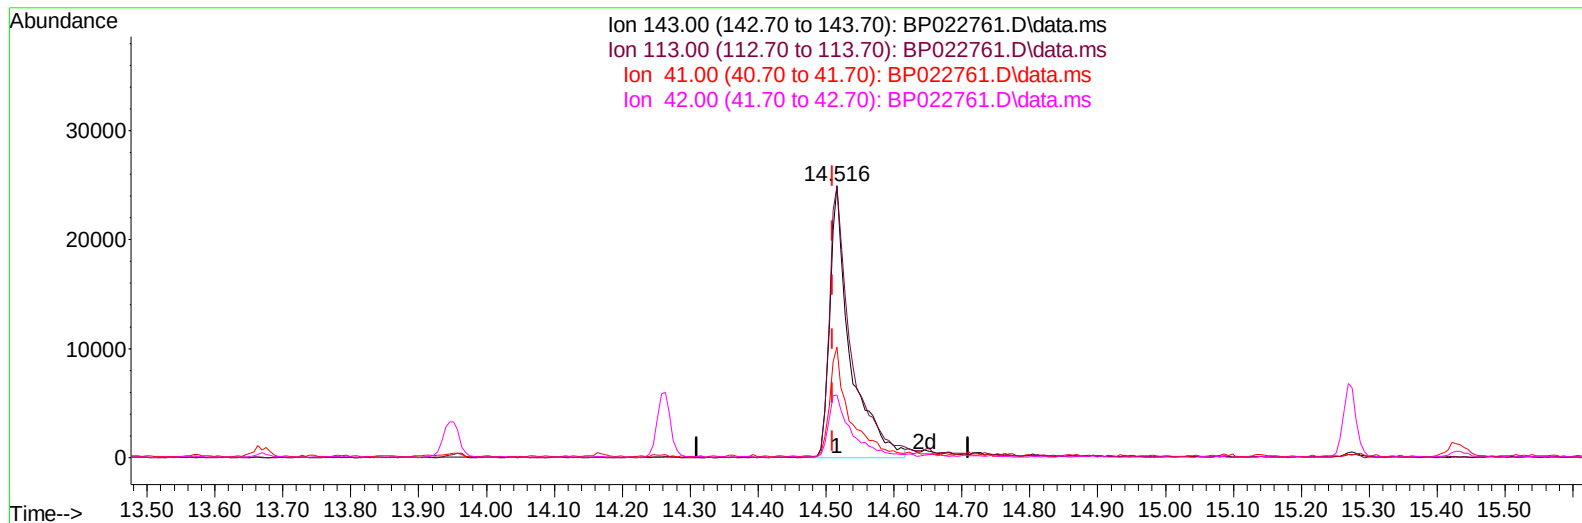

TIC: BP022761.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.516min (+ 0.006) 14.20 ng/ul m

response 51735

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	99.87
41.00	35.90	40.75
42.00	23.70	22.93

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022761.D
 Acq On : 31 Oct 2024 08:42
 Operator : RC/JU
 Sample : P4592-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7H07

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 01 01:42:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 30 10:56:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	88040	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	345058	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	273253	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.069	188	666825	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	740763	20.000	ng/ul	0.00
88) Perylene-d12	24.763	264	892888	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	6210	2.741	ng/uL	0.00
4) Pyridine-d5	3.599	84	55754	8.964	ng/ul	0.00
7) Phenol-d5	6.828	99	130192	17.568	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	72412	16.625	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	96530	18.357	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	110851	18.743	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	47236	17.804	ng/ul	0.00
24) 2-Nitrophenol-d4	9.487	143	58080	18.908	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.034	165	118972	18.224	ng/ul	0.00
31) 4-Chloroaniline-d4	10.534	131	129964	16.847	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	425965	19.620	ng/ul	0.00
49) Acenaphthylene-d8	13.946	160	453909	19.685	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	51735m	14.204	ng/ul	0.00
60) Fluorene-d10	15.275	176	393091	20.875	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	38646	8.812	ng/ul	0.03
73) Anthracene-d10	17.181	188	665455	21.214	ng/ul	0.01
81) Pyrene-d10	19.545	212	841854	21.491	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.533	264	1033161	21.666	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022761.D
Acq On : 31 Oct 2024 08:42
Operator : RC/JU
Sample : P4592-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H07

Manual IntegrationsAPPROVED

Quant Time: Nov 01 01:42:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

