




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022766.D
Acq On : 31 Oct 2024 12:05
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Quant Time: Oct 31 12:41:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

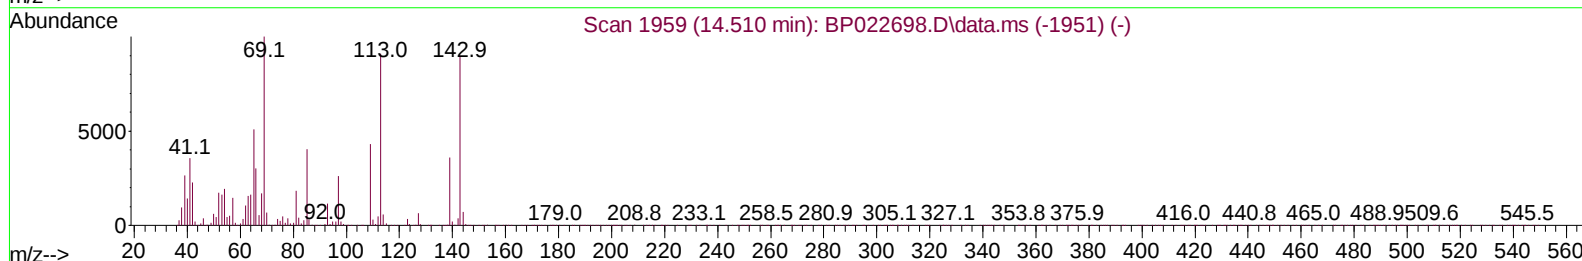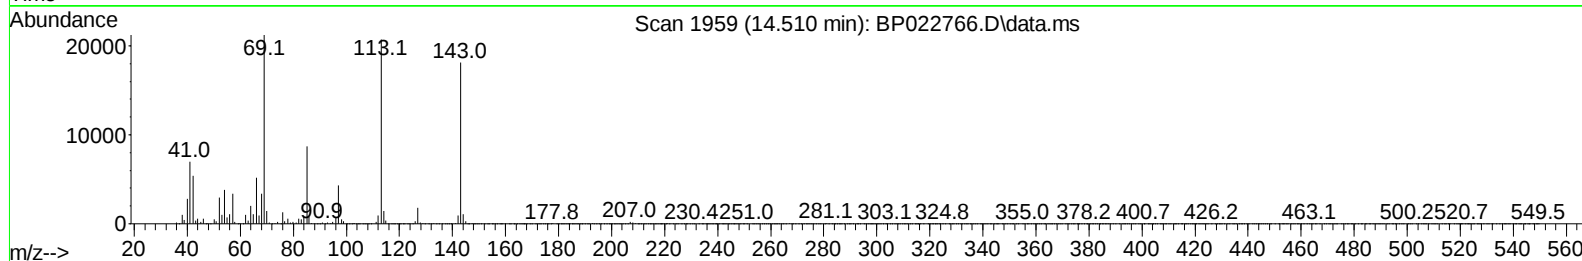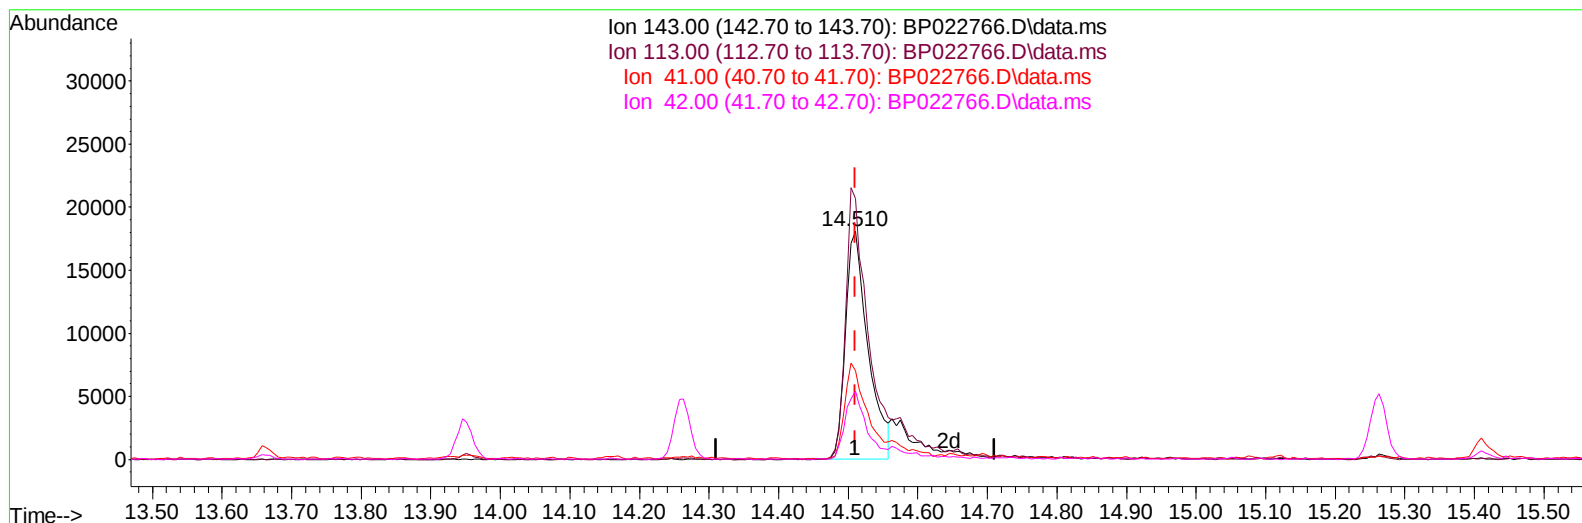

TIC: BP022766.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.510min (+ 0.000) 12.25 ng/u1

response 40723

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	114.27
41.00	35.90	38.71
42.00	23.70	29.89#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022766.D
Acq On : 31 Oct 2024 12:05
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

Quant Time: Oct 31 12:41:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

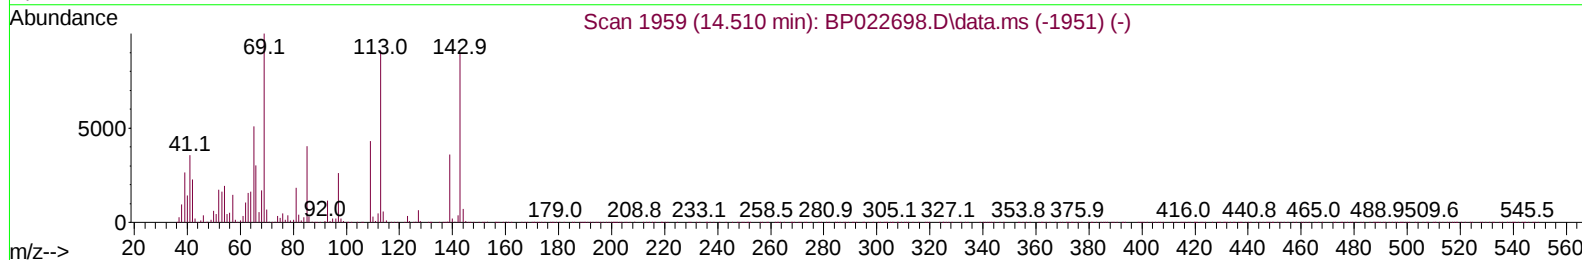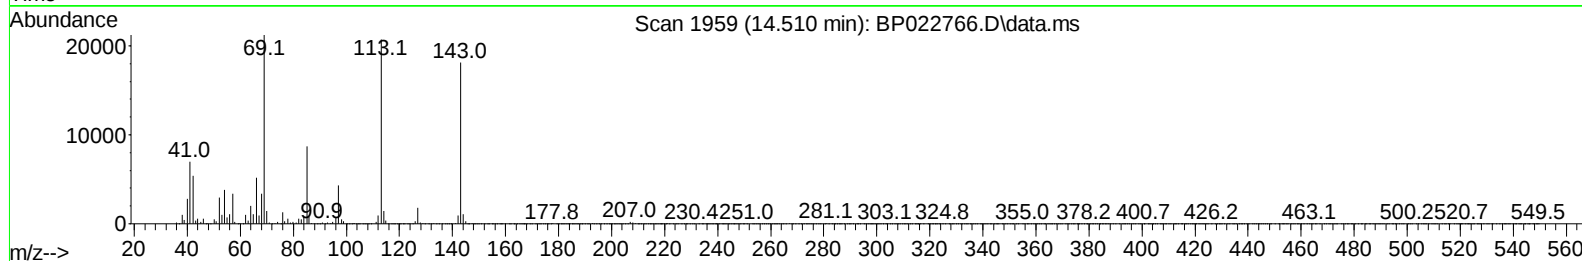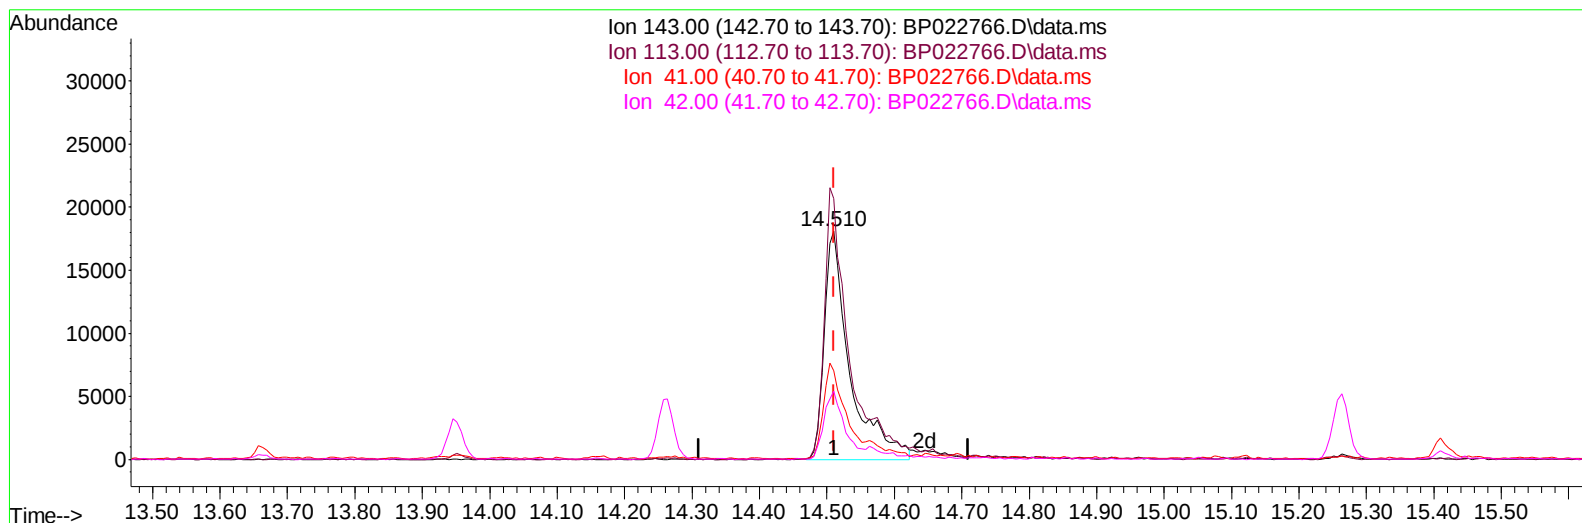

TIC: BP022766.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.510min (+ 0.000) 14.38 ng/ul m

response 47796

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	114.27
41.00	35.90	38.71
42.00	23.70	29.89#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022766.D
 Acq On : 31 Oct 2024 12:05
 Operator : RC/JU
 Sample : P4592-12
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7H20

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 01 01:55:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 30 10:56:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	81159	20.000	ng/ul	0.00
20) Naphthalene-d8	10.387	136	320512	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	249444	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.063	188	621452	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	719768	20.000	ng/ul	# 0.00
88) Perylene-d12	24.774	264	874042	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	6005	2.875	ng/uL	0.00
4) Pyridine-d5	3.593	84	63375	11.054	ng/ul	0.00
7) Phenol-d5	6.828	99	124871	18.278	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	67139	16.721	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	88426	18.241	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	102631	18.824	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	43100	17.489	ng/ul	0.00
24) 2-Nitrophenol-d4	9.487	143	52831	18.517	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.028	165	115232	19.002	ng/ul	0.00
31) 4-Chloroaniline-d4	10.534	131	123858	17.286	ng/ul	0.00
46) Dimethylphthalate-d6	13.663	166	394782	19.919	ng/ul	0.00
49) Acenaphthylene-d8	13.946	160	426952	20.283	ng/ul	0.00
54) 4-Nitrophenol-d4	14.510	143	47796m	14.375	ng/ul	0.00
60) Fluorene-d10	15.263	176	359132	20.892	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.410	200	36360	8.896	ng/ul	0.00
73) Anthracene-d10	17.169	188	627779	21.474	ng/ul	0.00
81) Pyrene-d10	19.545	212	812444	21.345	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.545	264	989303	21.194	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022766.D
Acq On : 31 Oct 2024 12:05
Operator : RC/JU
Sample : P4592-12
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7H20

Manual IntegrationsAPPROVED

Quant Time: Nov 01 01:55:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

