




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022802.D
 Acq On : 01 Nov 2024 13:23
 Operator : RC/JU
 Sample : P4630-17
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP11

Manual IntegrationsAPPROVED

Quant Time: Nov 01 16:09:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 30 10:56:39 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

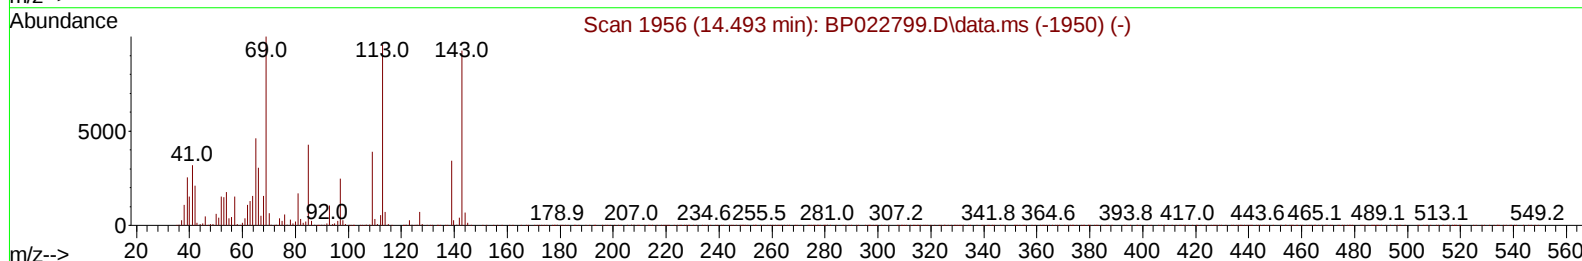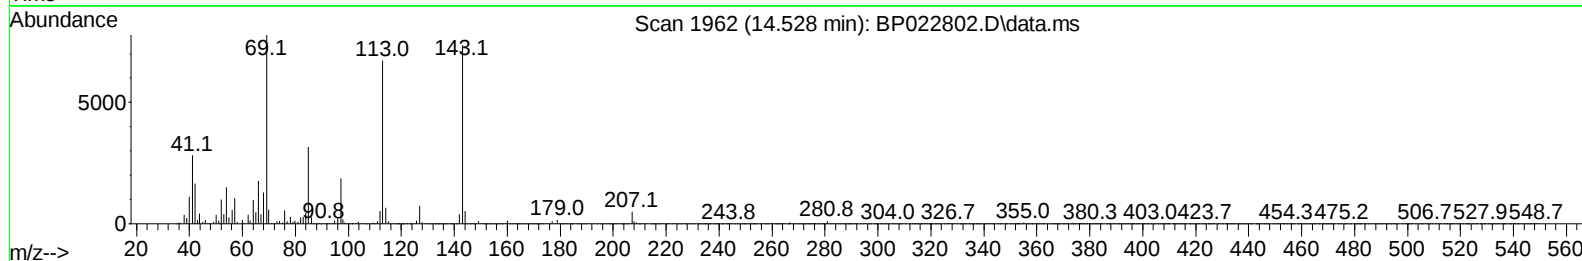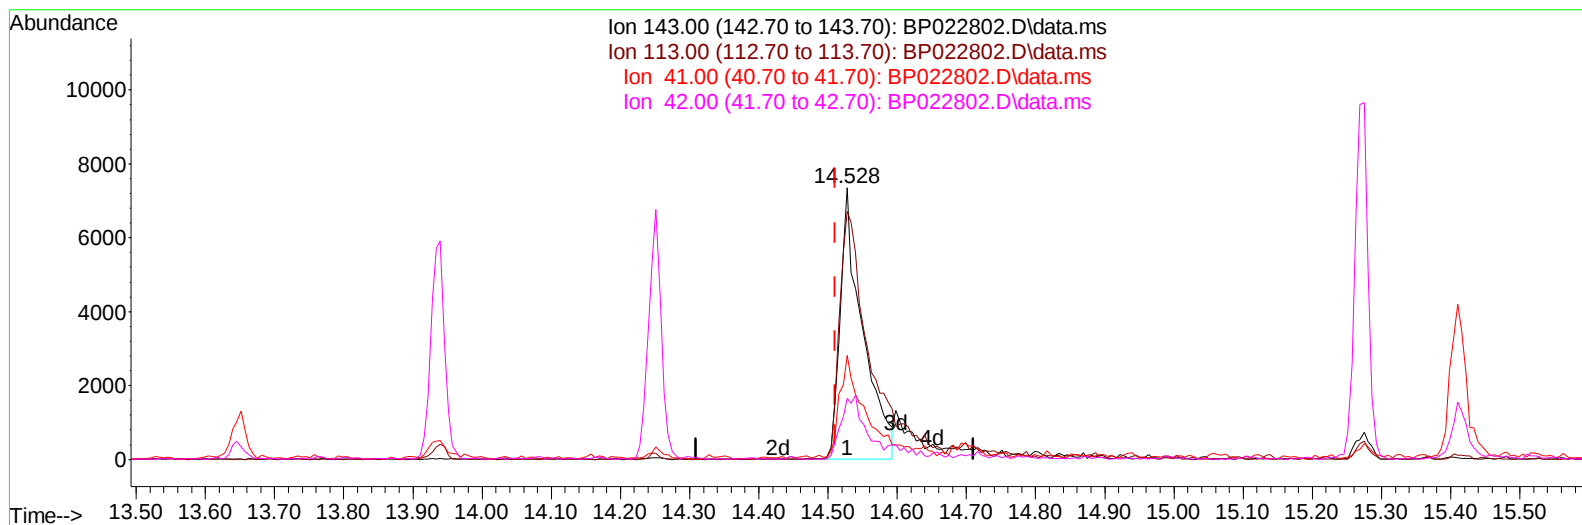

TIC: BP022802.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.018) 4.42 ng/u1

response 16463

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	91.36
41.00	35.90	38.36
42.00	23.70	22.51




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022802.D
Acq On : 01 Nov 2024 13:23
Operator : RC/JU
Sample : P4630-17
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP11

Manual IntegrationsAPPROVED

Quant Time: Nov 01 16:09:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

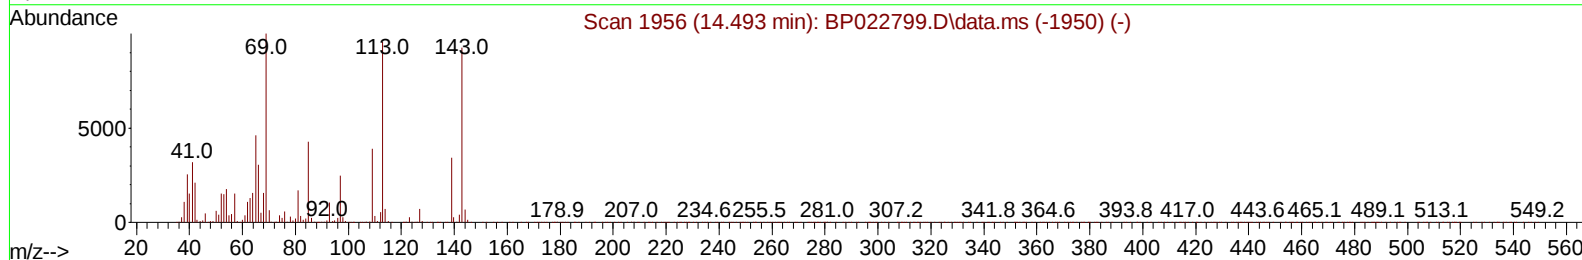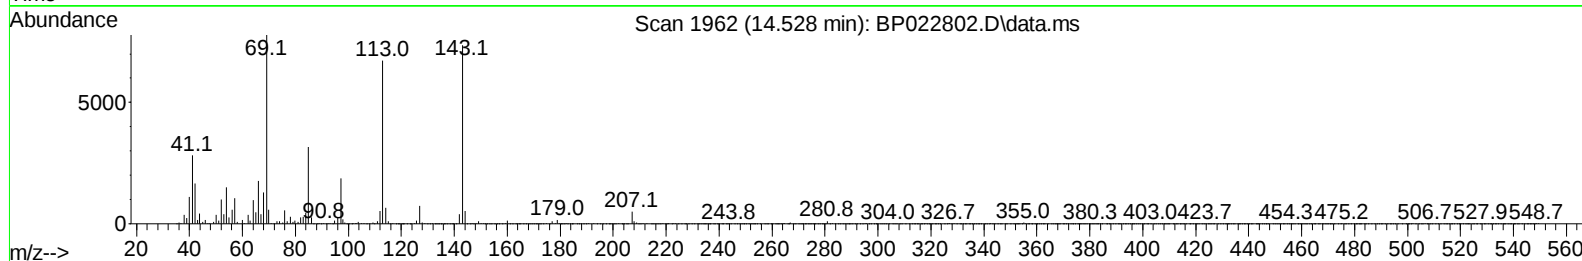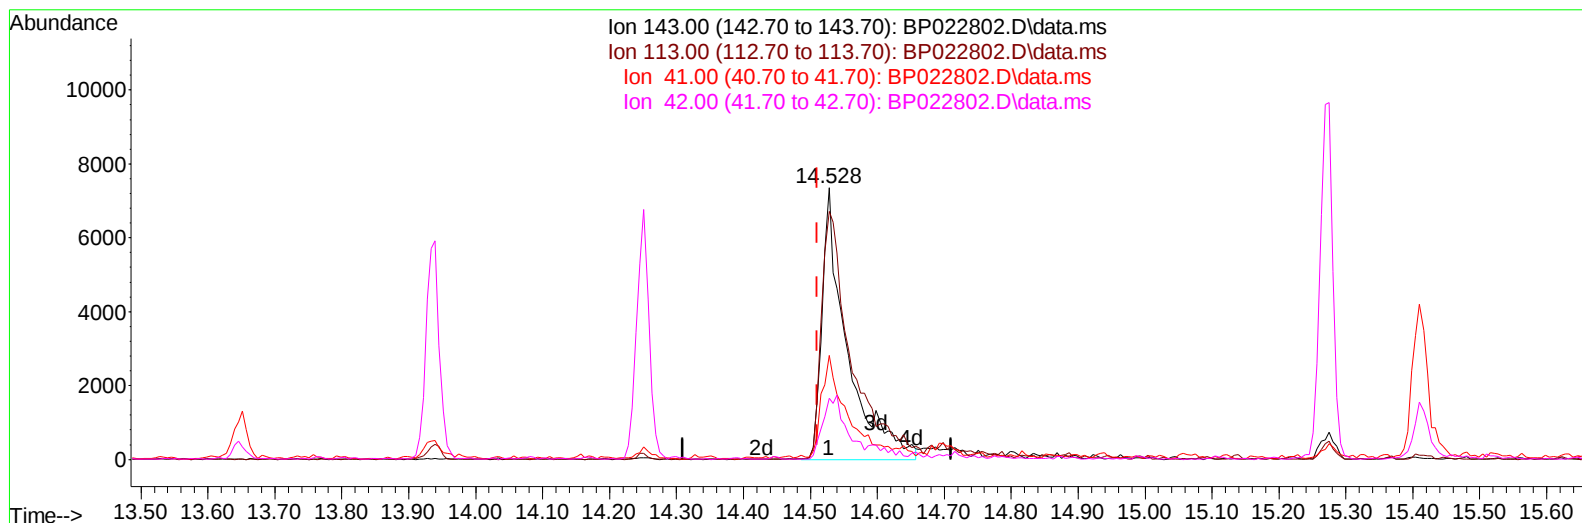

TIC: BP022802.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.018) 5.07 ng/ul m

response 18915

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	91.36
41.00	35.90	38.36
42.00	23.70	22.51

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022802.D
 Acq On : 01 Nov 2024 13:23
 Operator : RC/JU
 Sample : P4630-17
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP11

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 01 16:10:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 30 10:56:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	96904	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.381	136	355101	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.251	164	279666	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.057	188	678507	20.000	ng/ul	0.00
79) Chrysene-d12	21.504	240	764625	20.000	ng/ul	0.00
88) Perylene-d12	24.774	264	935430	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	7965	3.194	ng/uL	0.00
4) Pyridine-d5	3.593	84	43650	6.376	ng/ul	0.00
7) Phenol-d5	6.828	99	58963	7.228	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	108239	22.577	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	122837	21.223	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	107018	16.440	ng/ul	0.00
21) Nitrobenzene-d5	8.769	128	71386	26.145	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.487	143	83713	26.482	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.022	165	166932	24.847	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.534	131	140730	17.727	ng/ul	0.00
46) Dimethylphthalate-d6	13.651	166	593087	26.691	ng/ul	-0.01
49) Acenaphthylene-d8	13.940	160	612741	25.963	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.528	143	18915m	5.074	ng/ul	0.02
60) Fluorene-d10	15.275	176	527245	27.357	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	104259	23.364	ng/ul	0.00
73) Anthracene-d10	17.163	188	962858	30.166	ng/ul	0.00
81) Pyrene-d10	19.539	212	1242646	30.732	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.539	264	1568387	31.395	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022802.D
Acq On : 01 Nov 2024 13:23
Operator : RC/JU
Sample : P4630-17
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP11

Manual IntegrationsAPPROVED

Quant Time: Nov 01 16:10:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

