

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022745.D
 Acq On : 30 Oct 2024 21:12
 Operator : RC/JU
 Sample : P4493-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4F33

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Oct 31 22:47:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 30 10:56:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	92049	20.000	ng/u1	0.00
20) Naphthalene-d8	10.393	136	351901	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.251	164	272053	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.075	188	655679	20.000	ng/u1	0.01
79) Chrysene-d12	21.504	240	682880	20.000	ng/u1	# 0.00
88) Perylene-d12	24.763	264	829978	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	5860	2.474	ng/uL	0.00
4) Pyridine-d5	3.593	84	77305	11.888	ng/u1	0.00
7) Phenol-d5	6.828	99	117278	15.136	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	68658	15.076	ng/u1	0.00
11) 2-Chlorophenol-d4	7.181	132	91189	16.586	ng/u1	0.00
15) 4-Methylphenol-d8	8.340	113	104248	16.859	ng/u1	0.00
21) Nitrobenzene-d5	8.775	128	44307	16.375	ng/u1	0.00
24) 2-Nitrophenol-d4	9.493	143	54232	17.312	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.028	165	114772	17.238	ng/u1	0.00
31) 4-Chloroaniline-d4	10.540	131	89162	11.333	ng/u1	0.00
46) Dimethylphthalate-d6	13.675	166	391846	18.128	ng/u1	0.01
49) Acenaphthylene-d8	13.946	160	419770	18.284	ng/u1	0.00
54) 4-Nitrophenol-d4	14.516	143	42387	11.689	ng/u1	0.00
60) Fluorene-d10	15.269	176	352787	18.817	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.422	200	34063m	7.899	ng/u1	0.02
73) Anthracene-d10	17.169	188	590004	19.128	ng/u1	0.00
81) Pyrene-d10	19.539	212	741261	20.527	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.533	264	868662	19.598	ng/u1	0.01
Target Compounds						
					Qvalue	
72) Phenanthrene	17.116	178	45581	1.299	ng/u1	96
80) Fluoranthene	19.192	202	99676	2.401	ng/u1#	96
82) Pyrene	19.569	202	87241	1.961	ng/u1	99
87) Chrysene	21.551	228	49025	1.104	ng/u1	94
90) Benzo(b)fluoranthene	23.733	252	70683	1.353	ng/u1	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022745.D
Acq On : 30 Oct 2024 21:12
Operator : RC/JU
Sample : P4493-04
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A4F33

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024


Quant Time: Oct 31 22:47:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

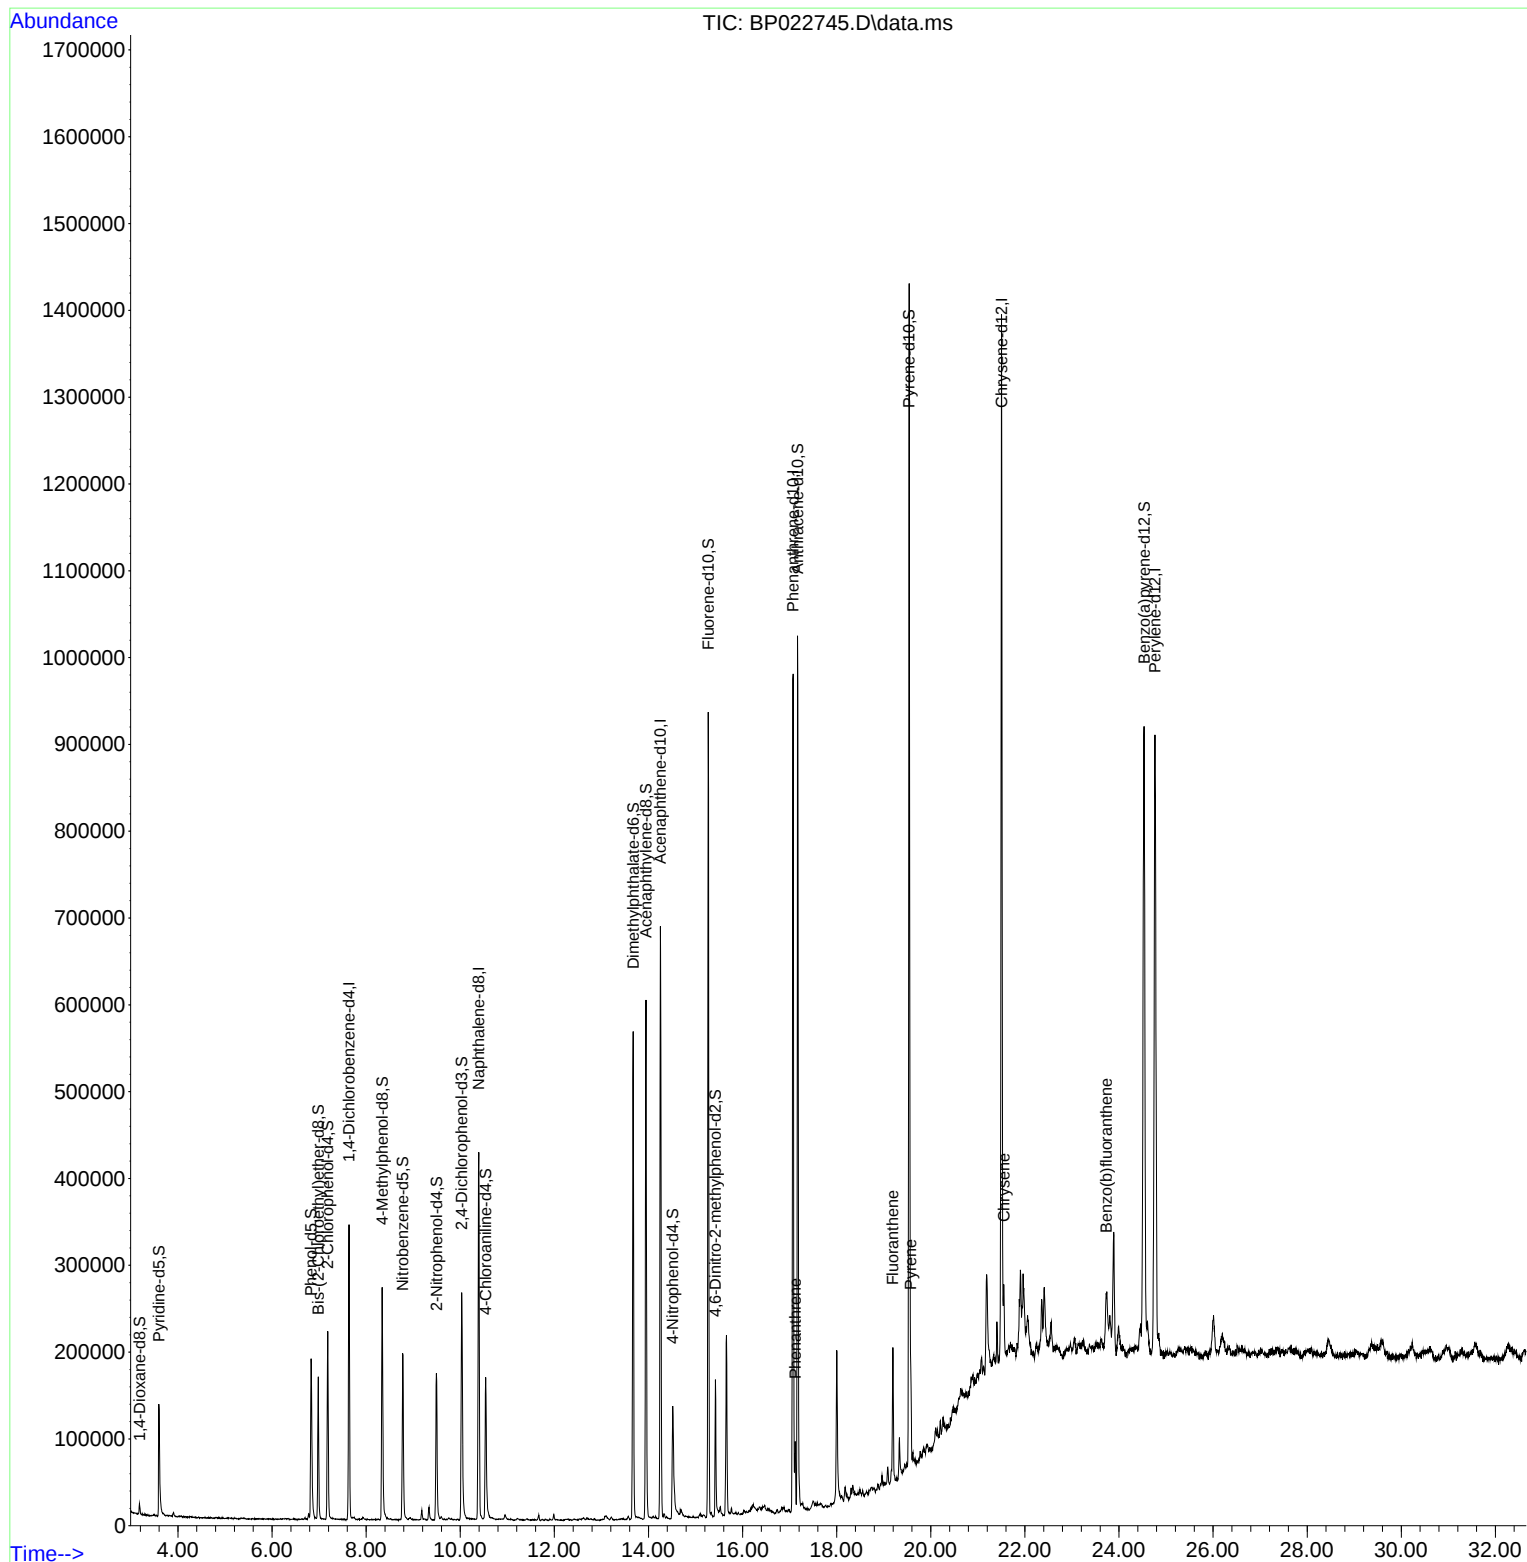

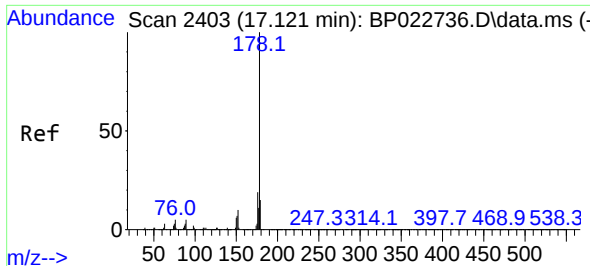

#72
Phenanthrene
Concen: 1.299 ng/ul
RT: 17.116 min Scan# 2402
Delta R.T. 0.012 min
Lab File: BP022745.D
Acq: 30 Oct 2024 21:12




Instrument :
BNA_P
ClientSampleId :
A4F33

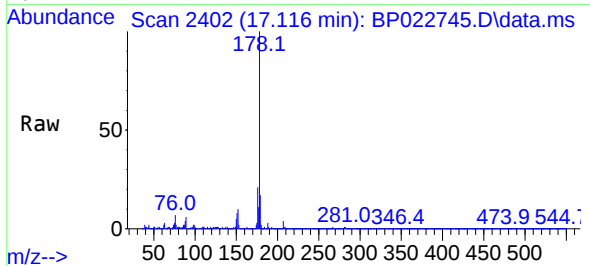

Tgt Ion:178 Resp: 4558
Ion Ratio Lower Upper
178 100
179 17.2 12.2 18.4
176 21.1 15.7 23.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

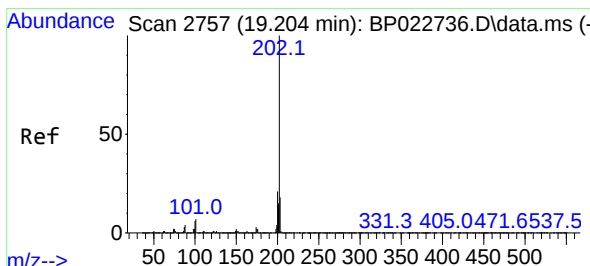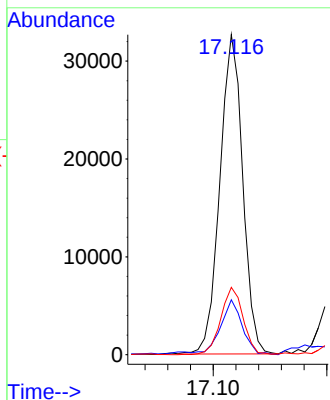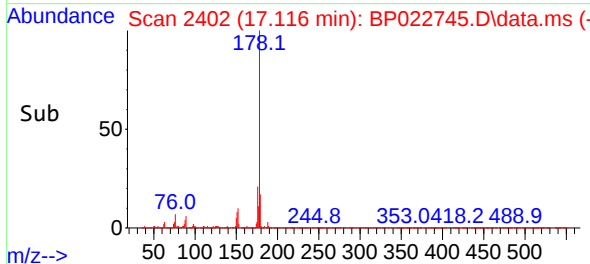

#80
Fluoranthene
Concen: 2.401 ng/ul
RT: 19.192 min Scan# 2755
Delta R.T. 0.000 min
Lab File: BP022745.D
Acq: 30 Oct 2024 21:12

Tgt Ion:202 Resp: 99676
Ion Ratio Lower Upper
202 100
101 6.0 5.8 8.8
100 4.3 4.5 6.7

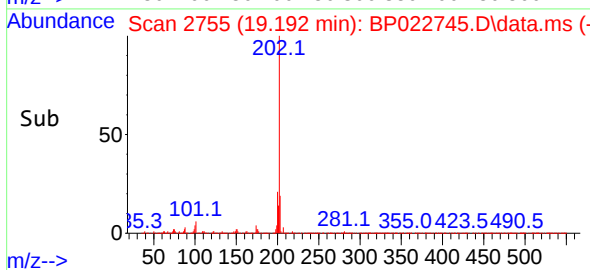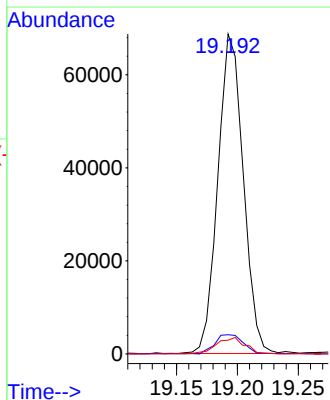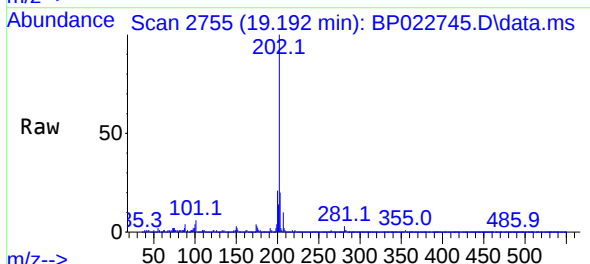

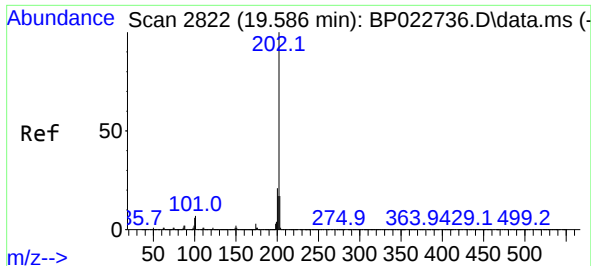





#82
Pyrene
Concen: 1.961 ng/ul
RT: 19.569 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP022745.D
Acq: 30 Oct 2024 21:12

Instrument :
BNA_P
ClientSampleId :
A4F33

Tgt Ion:	202	Resp:	8724
Ion Ratio	Lower	Upper	
202	100		
101	7.9	6.7	10.1
100	7.6	5.8	8.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

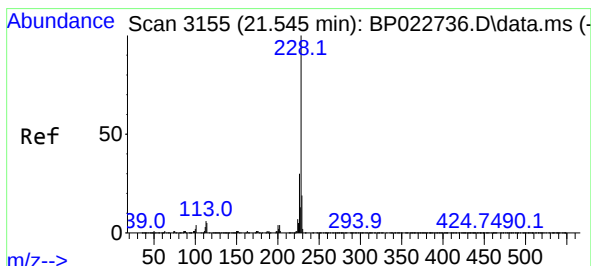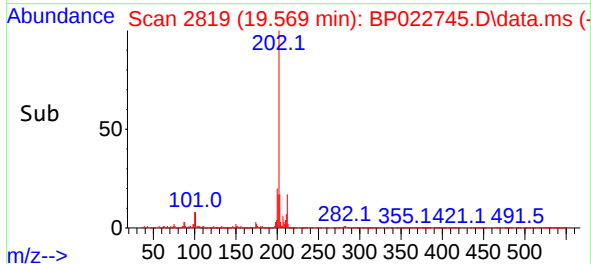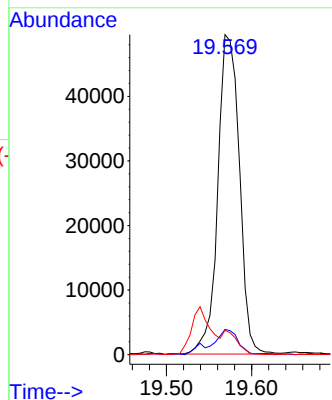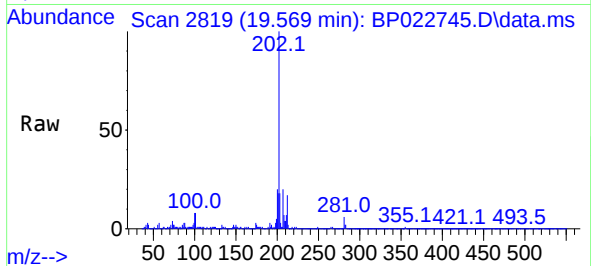

#87
Chrysene
Concen: 1.104 ng/ul
RT: 21.551 min Scan# 3156
Delta R.T. 0.000 min
Lab File: BP022745.D
Acq: 30 Oct 2024 21:12


Tgt Ion:	228	Resp:	49025
Ion Ratio	Lower	Upper	
228	100		
226	32.5	23.8	35.8
229	23.1	15.5	23.3

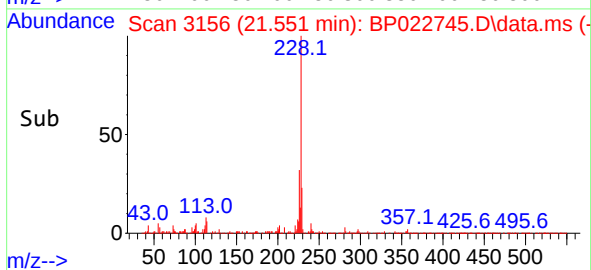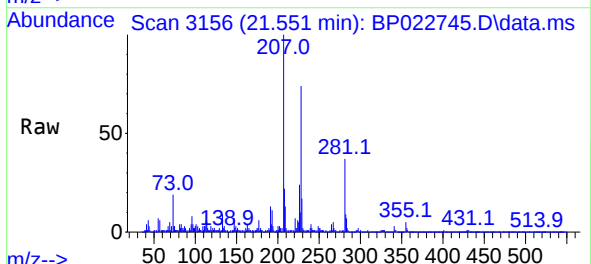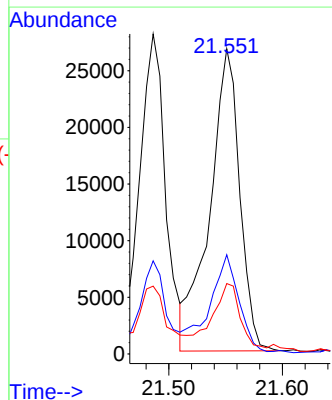

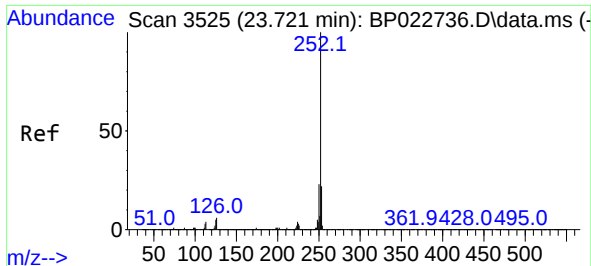

#90
Benzo(b)fluoranthene
Concen: 1.353 ng/ul
RT: 23.733 min Scan# 31
Delta R.T. 0.012 min
Lab File: BP022745.D
Acq: 30 Oct 2024 21:12

Instrument :
BNA_P
ClientSampleId :
A4F33

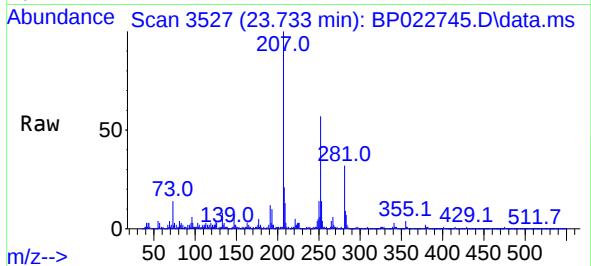

Tgt Ion: 252 Resp: 7068
Ion Ratio Lower Upper
252 100
253 24.6 17.8 26.8
125 6.6 5.0 7.4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

