

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022788.D
 Acq On : 01 Nov 2024 03:52
 Operator : RC/JU
 Sample : P4630-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP04

Quant Time: Nov 01 06:52:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 30 10:56:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	93658	20.000	ng/u1	0.00
20) Naphthalene-d8	10.387	136	353971	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.263	164	269536	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.063	188	651330	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	804334	20.000	ng/u1	0.00
88) Perylene-d12	24.768	264	937328	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	8087	3.355	ng/uL	0.00
4) Pyridine-d5	3.599	84	51151	7.731	ng/u1	0.00
7) Phenol-d5	6.834	99	58713	7.447	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	128805	27.798	ng/u1	0.00
11) 2-Chlorophenol-d4	7.175	132	148889	26.615	ng/u1	0.00
15) 4-Methylphenol-d8	8.340	113	117061	18.606	ng/u1	0.00
21) Nitrobenzene-d5	8.775	128	83582	30.710	ng/u1	0.00
24) 2-Nitrophenol-d4	9.487	143	103561	32.866	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.028	165	205182	30.637	ng/u1	0.00
31) 4-Chloroaniline-d4	10.528	131	171881	21.720	ng/u1	-0.01
46) Dimethylphthalate-d6	13.651	166	671521	31.357	ng/u1	-0.01
49) Acenaphthylene-d8	13.945	160	711670	31.288	ng/u1	0.00
54) 4-Nitrophenol-d4	14.528	143	20119	5.600	ng/u1	0.02
60) Fluorene-d10	15.275	176	599441	32.272	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	106444	24.849	ng/u1	0.00
73) Anthracene-d10	17.163	188	1050396	34.282	ng/u1	0.00
81) Pyrene-d10	19.551	212	1399326	32.898	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.551	264	1764822	35.255	ng/u1	0.03


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.211	88	13428	5.182	ng/uL#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022788.D
Acq On : 01 Nov 2024 03:52
Operator : RC/JU
Sample : P4630-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP04

Quant Time: Nov 01 06:52:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

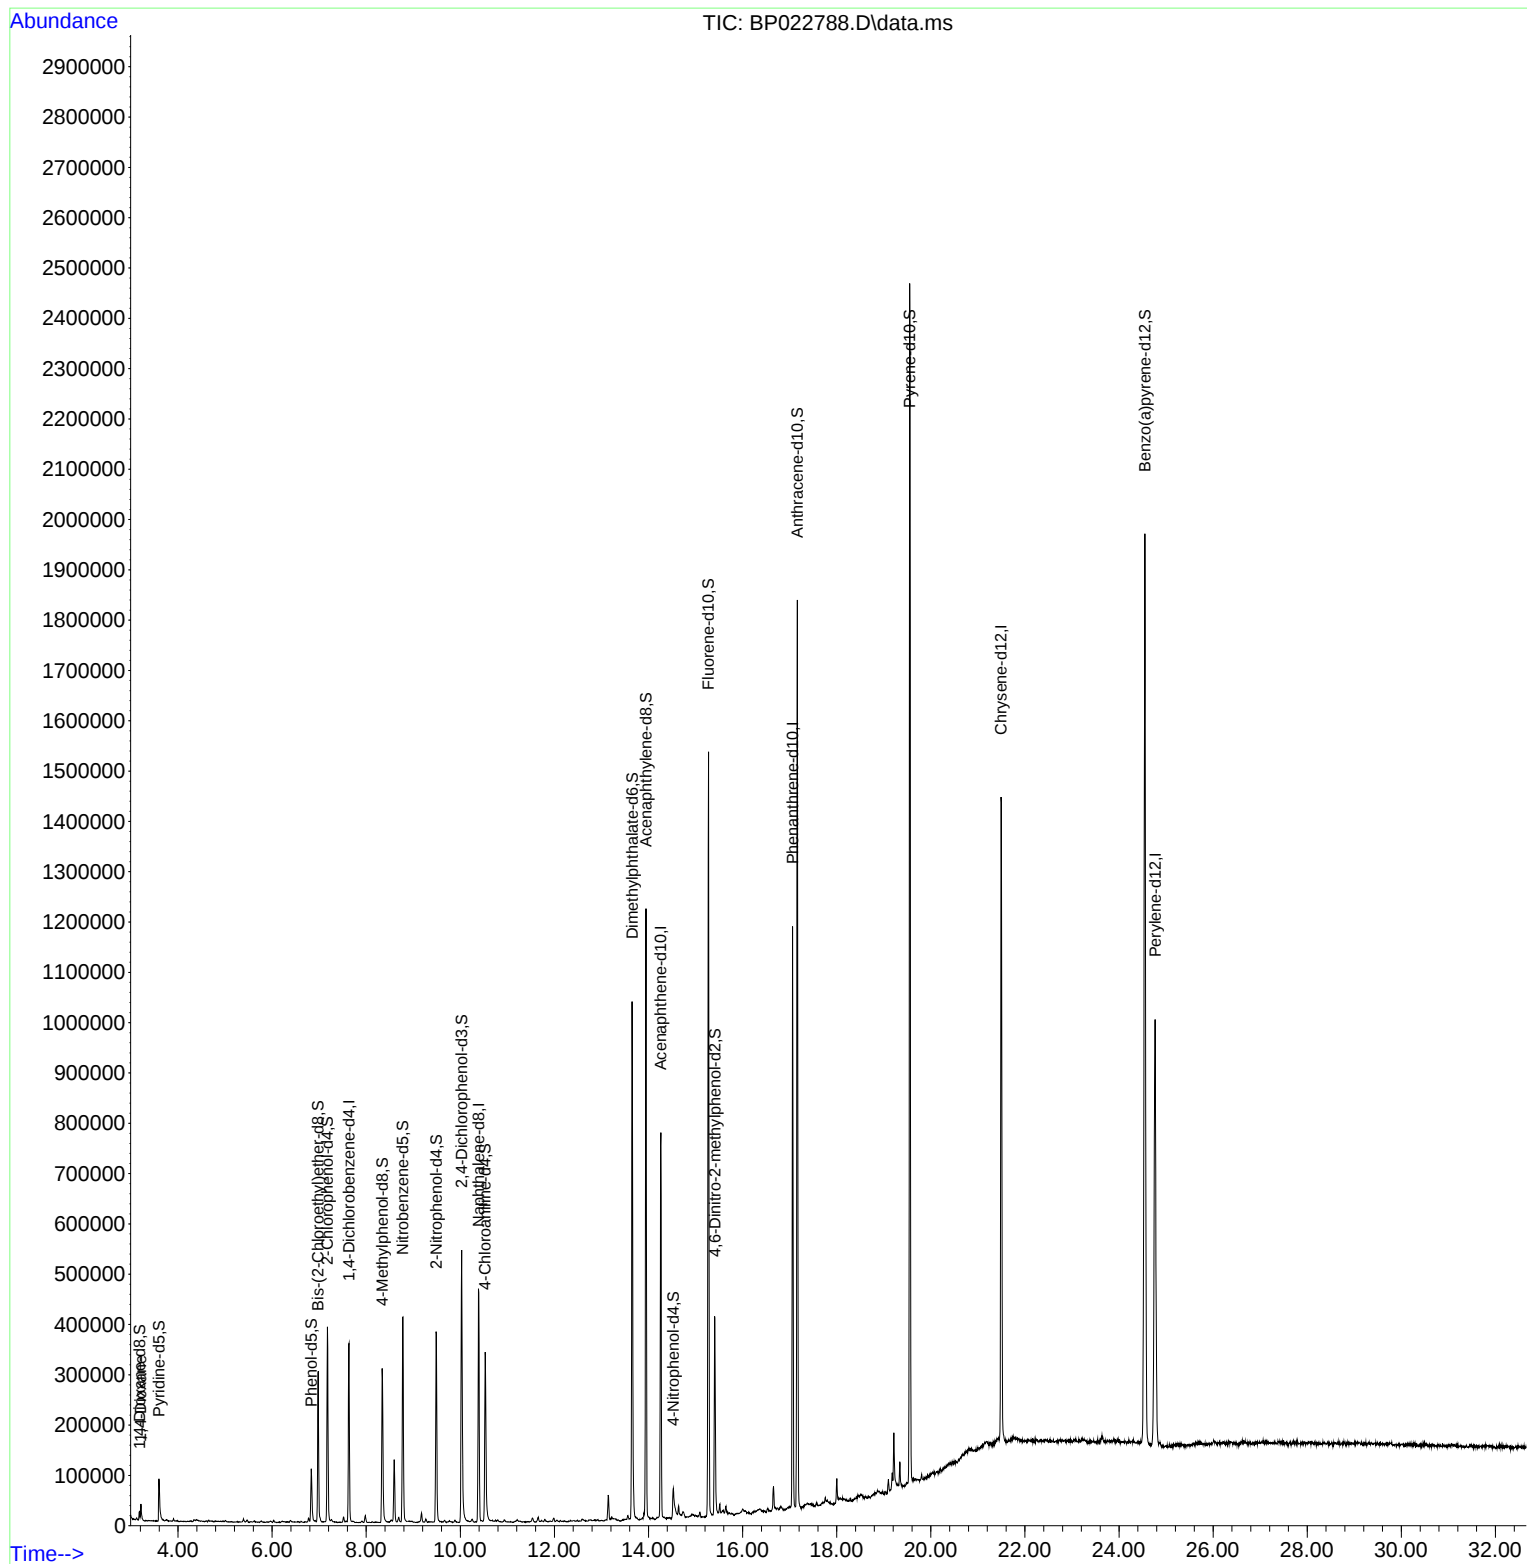

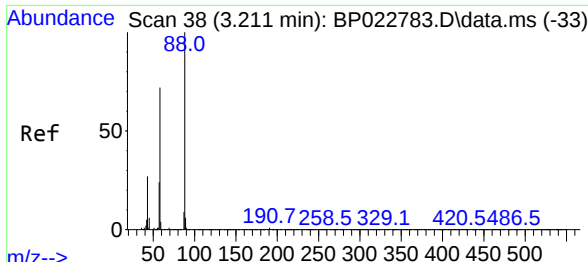

#2
1,4-Dioxane
Concen: 5.182 ng/uL
RT: 3.211 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP022788.D
Acq: 01 Nov 2024 03:52

Instrument :
BNA_P
ClientSampleId :
GCP04

Tgt Ion: 88 Resp: 13428

Ion	Ratio	Lower	Upper
88	100		
43	43.4	22.3	33.5#
58	73.1	54.7	82.1

