

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022752.D
 Acq On : 31 Oct 2024 02:37
 Operator : RC/JU
 Sample : PB164506BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK506

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	40	rVB	21959	30004	1.09%	0.112%
2	3.593	99	103	120	rBV	262737	430094	15.70%	1.603%
3	3.905	151	156	161	rBV	39911	55078	2.01%	0.205%
4	6.781	640	645	647	rBV	4355	6043	0.22%	0.023%
5	6.834	647	654	667	rVV	323261	572709	20.90%	2.134%
6	6.981	673	679	692	rVB	251527	399545	14.58%	1.489%
7	7.181	705	713	724	rBV	348654	577196	21.06%	2.151%
8	7.634	782	790	802	rBV	365386	585776	21.38%	2.183%
9	8.340	903	910	928	rBV	409522	734872	26.82%	2.738%
10	8.781	977	985	998	rBV	350872	570804	20.83%	2.127%
11	9.181	1046	1053	1058	rBV3	7907	12843	0.47%	0.048%
12	9.493	1099	1106	1120	rBV	311432	510206	18.62%	1.901%
13	10.028	1188	1197	1218	rBV	415042	818483	29.87%	3.050%
14	10.387	1249	1258	1270	rVB	468685	812563	29.65%	3.028%
15	10.534	1276	1283	1299	rBV	399407	719046	26.24%	2.679%
16	11.657	1469	1474	1479	rBV3	6770	10517	0.38%	0.039%
17	11.987	1524	1530	1537	rBV3	6363	12382	0.45%	0.046%
18	13.210	1734	1738	1744	rVB9	1436	3031	0.11%	0.011%
19	13.669	1809	1816	1830	rBV	774831	1206860	44.04%	4.497%
20	13.934	1854	1861	1878	rBV	827260	1400349	51.10%	5.218%
21	14.246	1907	1914	1924	rBV	712017	1236538	45.12%	4.607%
22	14.498	1951	1957	1980	rBV	244316	578105	21.10%	2.154%
23	15.257	2080	2086	2096	rBV	1477528	1843473	67.27%	6.869%
24	15.410	2104	2112	2123	rBV	229441	367251	13.40%	1.368%
25	15.516	2128	2130	2136	rVB2	8217	10144	0.37%	0.038%
26	16.063	2220	2223	2228	rVB7	2652	3316	0.12%	0.012%
27	16.534	2299	2303	2306	rBV6	2790	4581	0.17%	0.017%
28	16.728	2332	2336	2339	rBV5	2254	3168	0.12%	0.012%
29	16.857	2352	2358	2362	rBV5	2408	4978	0.18%	0.019%
30	17.057	2386	2392	2402	rBV	1256168	1704640	62.21%	6.352%
31	17.157	2402	2409	2429	rVB2	1281994	2114828	77.18%	7.880%
32	17.369	2442	2445	2446	rBV3	3660	3931	0.14%	0.015%
33	17.645	2488	2492	2497	rVB8	3811	5874	0.21%	0.022%
34	18.004	2548	2553	2557	rBV7	5075	8174	0.30%	0.030%
35	19.098	2736	2739	2745	rVB2	22360	28364	1.04%	0.106%
36	19.169	2747	2751	2758	rVB	22952	30133	1.10%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022752.D
Acq On : 31 Oct 2024 02:37
Operator : RC/JU
Sample : PB164506BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK506

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	19.545	2809	2815	2826	rBV	1950417	2634502	96.14%	9.816%
38	21.498	3141	3147	3157	rVB2	1281359	2040489	74.46%	7.603%
39	24.521	3652	3661	3674	rVB	1032679	2740251	100.00%	10.210%
40	24.757	3692	3701	3714	rVB2	745809	2006973	73.24%	7.478%


Sum of corrected areas: 26838114

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022752.D
Acq On : 31 Oct 2024 02:37
Operator : RC/JU
Sample : PB164506BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK506

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

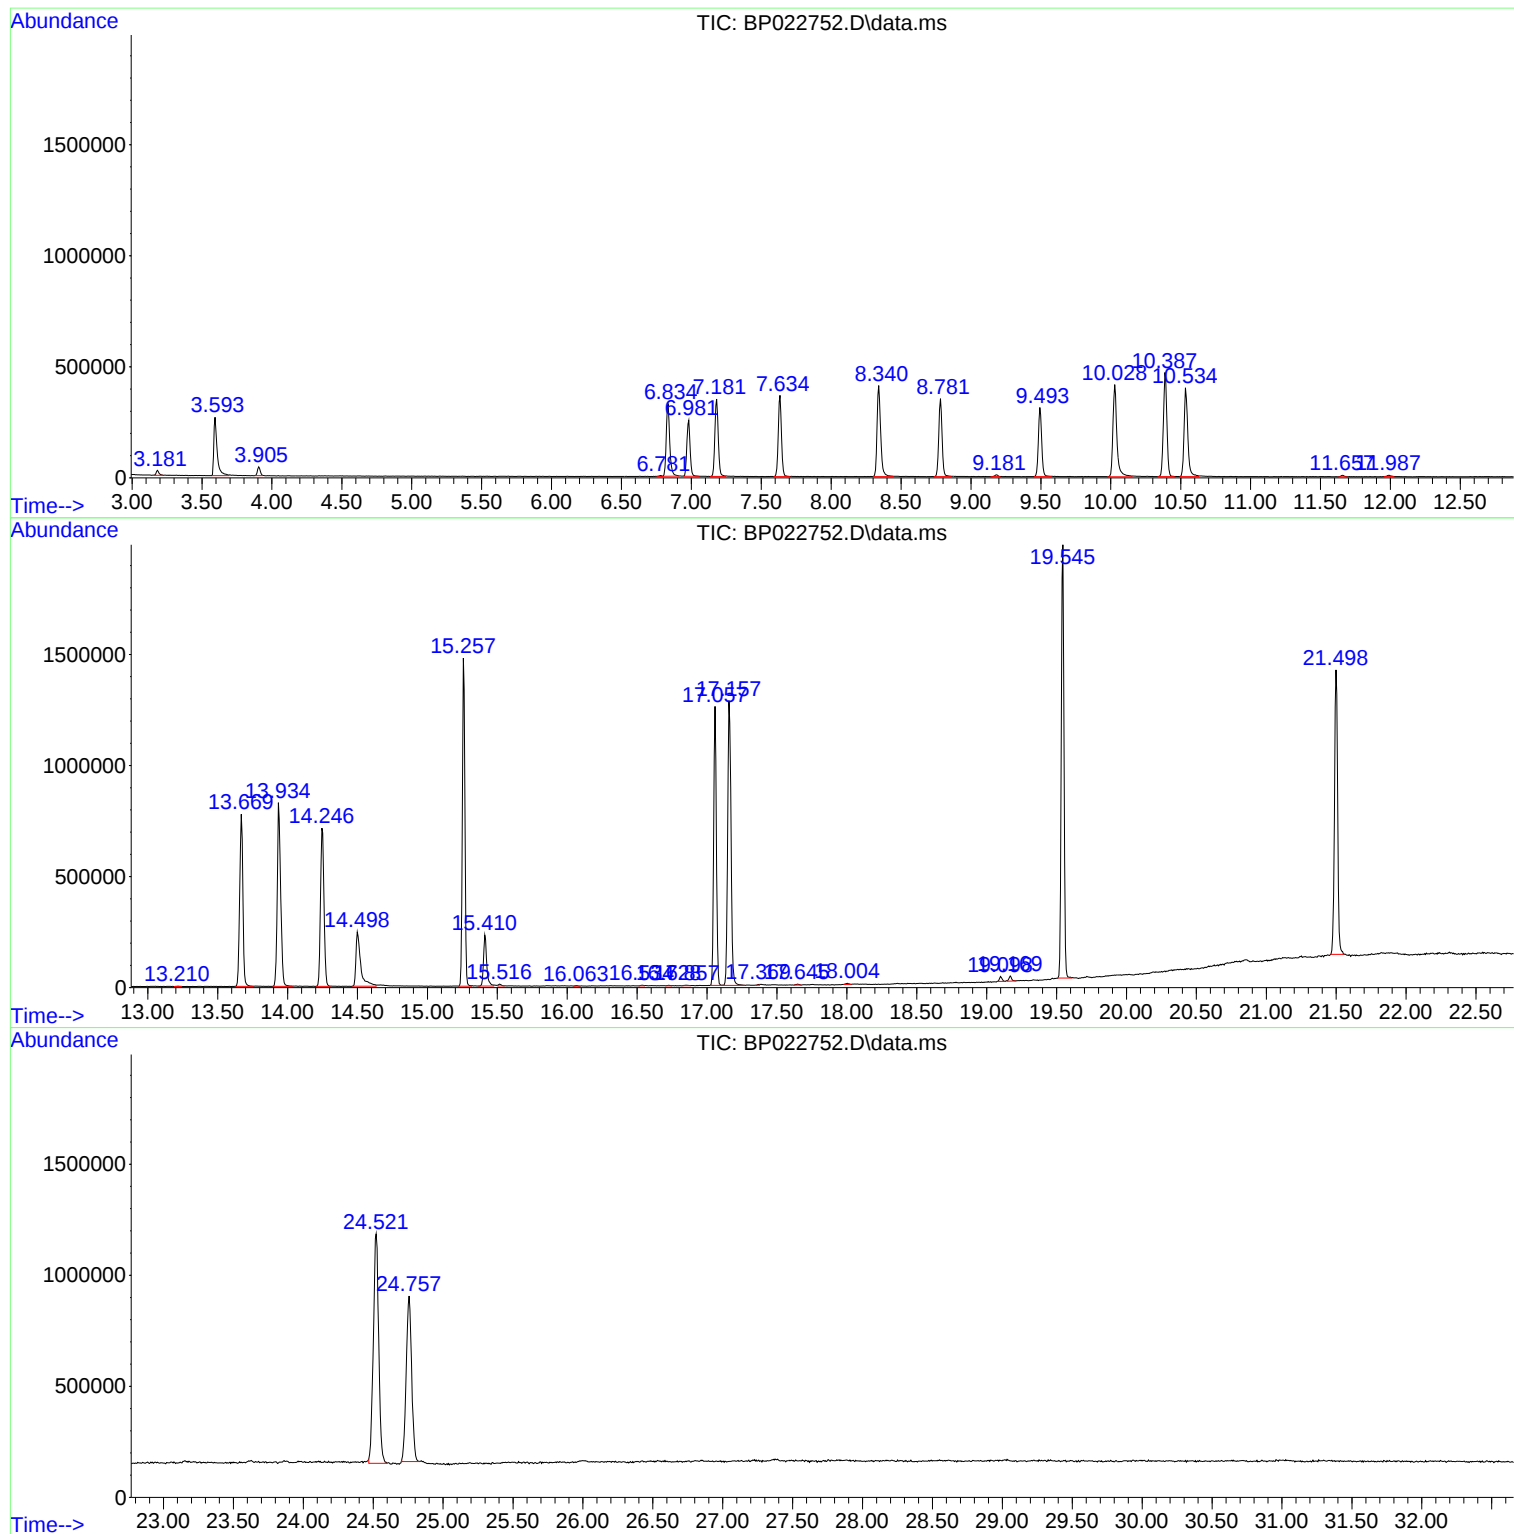

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022752.D
Acq On : 31 Oct 2024 02:37
Operator : RC/JU
Sample : PB164506BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK506

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022752.D
Acq On : 31 Oct 2024 02:37
Operator : RC/JU
Sample : PB164506BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK506

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc