

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022769.D
 Acq On : 31 Oct 2024 14:10
 Operator : RC/JU
 Sample : PB164546BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK546

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022769.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	26	31	42	rVB	21931	32858	1.19%	0.128%
2	3.575	96	100	122	rBV	252643	430002	15.54%	1.673%
3	3.893	150	154	159	rVB2	5641	8009	0.29%	0.031%
4	6.763	636	642	644	rBV4	2218	3386	0.12%	0.013%
5	6.810	644	650	668	rVV	348546	572670	20.70%	2.229%
6	6.958	669	675	685	rVB	249371	391649	14.16%	1.524%
7	7.157	702	709	728	rBV	349046	573782	20.74%	2.233%
8	7.616	780	787	798	rBB	327758	520137	18.80%	2.024%
9	8.322	900	907	920	rBV	394401	717746	25.94%	2.793%
10	8.757	975	981	996	rBV	340781	567060	20.50%	2.207%
11	9.469	1095	1102	1113	rBV	293841	506401	18.30%	1.971%
12	9.546	1113	1115	1122	rVB6	1960	3756	0.14%	0.015%
13	10.022	1187	1196	1218	rBV	426003	803043	29.03%	3.125%
14	10.375	1248	1256	1265	rBV	389469	708361	25.61%	2.757%
15	10.516	1273	1280	1298	rBV	358357	704125	25.45%	2.740%
16	11.993	1524	1531	1538	rBV3	5832	13027	0.47%	0.051%
17	13.657	1808	1814	1827	rBV	919938	1205138	43.56%	4.690%
18	13.951	1856	1864	1877	rBV	1010614	1377357	49.79%	5.360%
19	14.263	1908	1917	1928	rBV	774024	1060762	38.34%	4.128%
20	14.510	1952	1959	1979	rBV	212895	568928	20.56%	2.214%
21	15.269	2081	2088	2102	rBV	1090997	1793484	64.83%	6.979%
22	15.404	2106	2111	2125	rBV	268324	453675	16.40%	1.765%
23	15.504	2125	2128	2133	rVB4	5478	8488	0.31%	0.033%
24	16.075	2220	2225	2228	rBV7	1879	3026	0.11%	0.012%
25	16.733	2333	2337	2338	rBV3	2026	2769	0.10%	0.011%
26	16.845	2351	2356	2359	rBV6	2587	4382	0.16%	0.017%
27	17.069	2386	2394	2405	rBV	895729	1428998	51.65%	5.561%
28	17.169	2405	2411	2422	rVV	1730487	2108117	76.20%	8.204%
29	17.422	2450	2454	2457	rBV6	2590	3712	0.13%	0.014%
30	17.492	2461	2466	2469	rBV7	2740	4705	0.17%	0.018%
31	18.010	2552	2554	2560	rVB7	3348	5088	0.18%	0.020%
32	19.092	2734	2738	2742	rVB3	18483	25200	0.91%	0.098%
33	19.175	2748	2752	2759	rBV2	17607	29226	1.06%	0.114%
34	19.551	2810	2816	2827	rBV	1832073	2699477	97.58%	10.505%
35	21.504	3143	3148	3156	rBV	1186952	1807566	65.34%	7.034%
36	24.551	3656	3666	3680	rVB	1004625	2766488	100.00%	10.766%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022769.D
Acq On : 31 Oct 2024 14:10
Operator : RC/JU
Sample : PB164546BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.774	3695	3704	3716	rVB	746154	1784255	64.50%	6.943%
----	--------	------	------	------	-----	--------	---------	--------	--------


Sum of corrected areas: 25696853

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022769.D
Acq On : 31 Oct 2024 14:10
Operator : RC/JU
Sample : PB164546BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

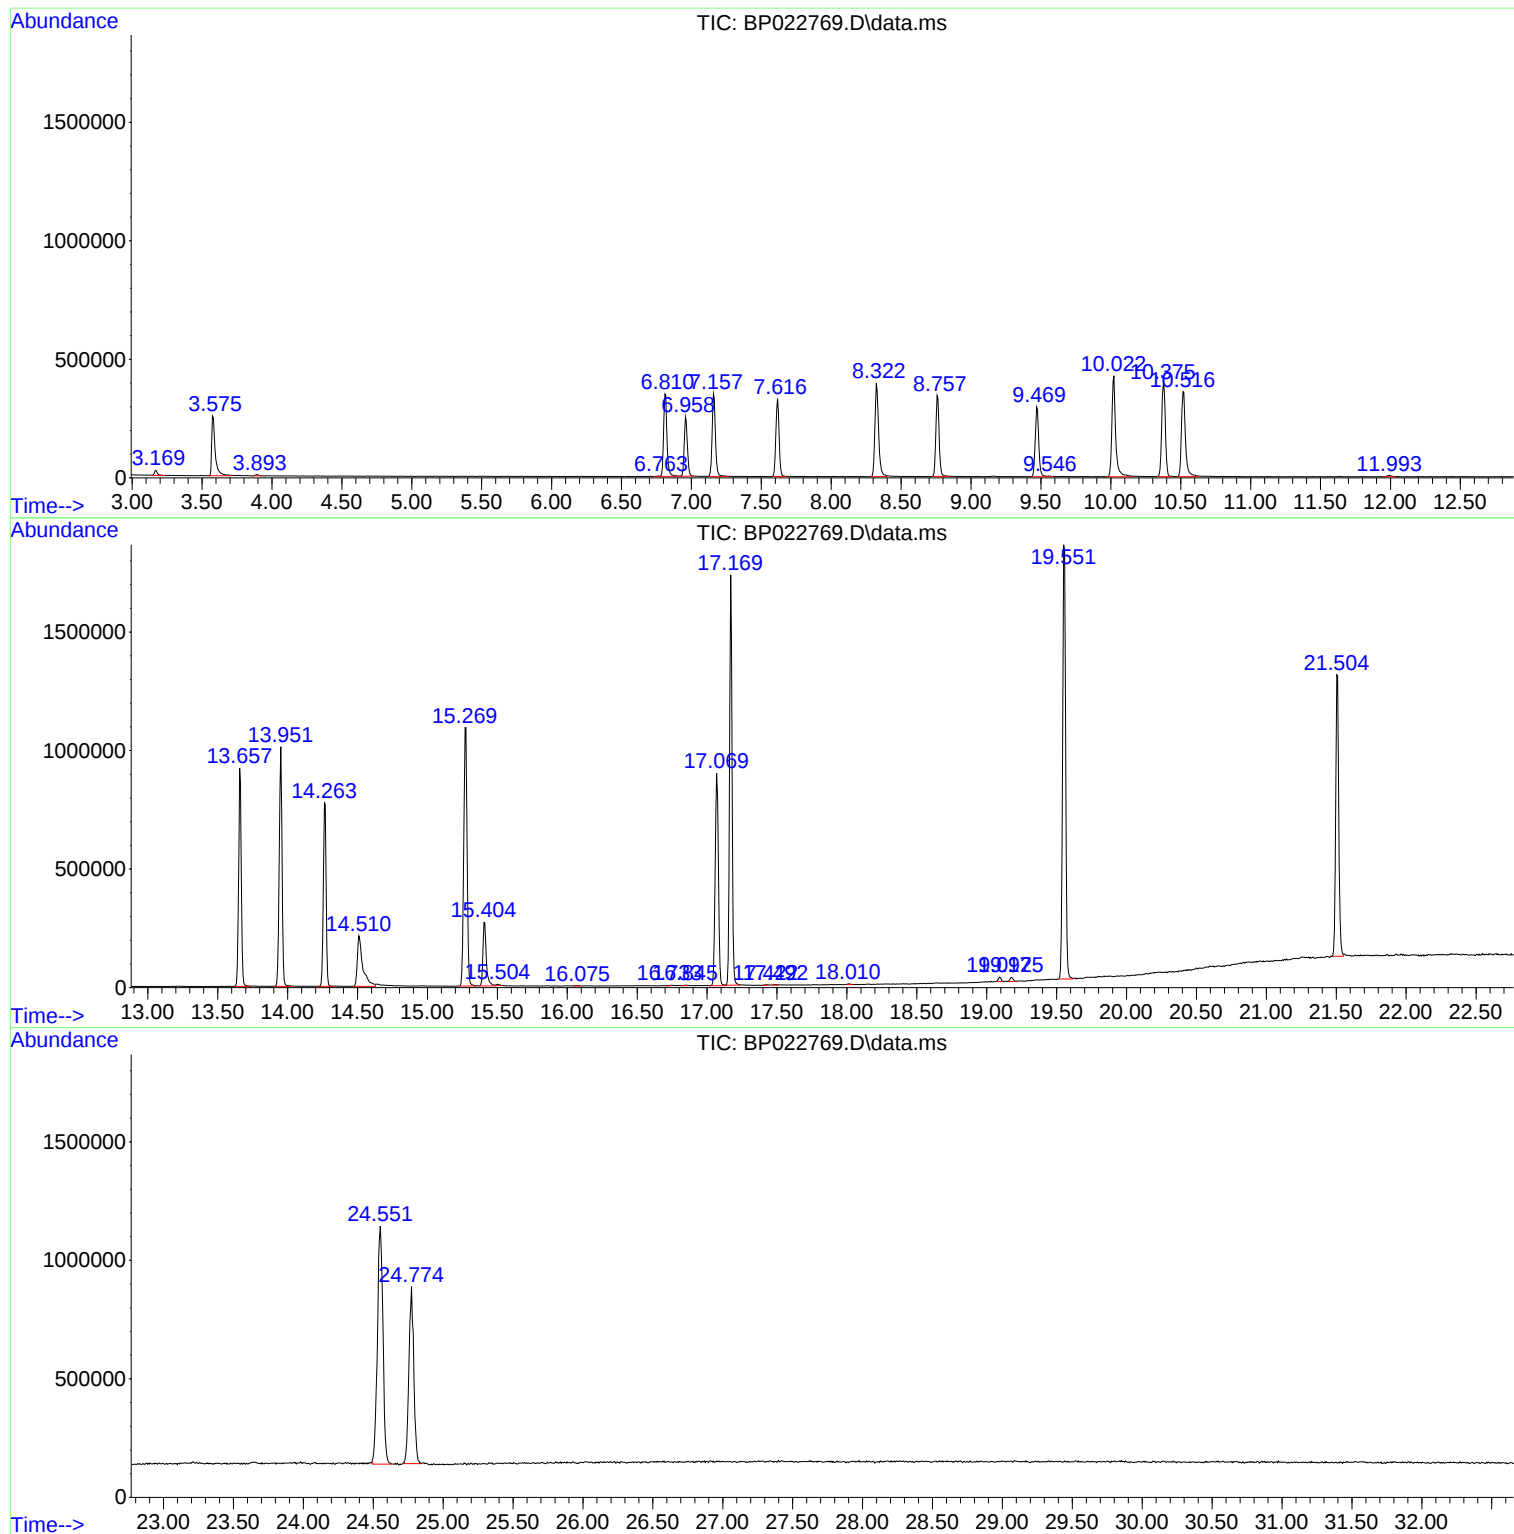

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022769.D
Acq On : 31 Oct 2024 14:10
Operator : RC/JU
Sample : PB164546BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022769.D
Acq On : 31 Oct 2024 14:10
Operator : RC/JU
Sample : PB164546BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc