

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022774.D
 Acq On : 31 Oct 2024 17:40
 Operator : RC/JU
 Sample : P4630-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022774.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	36	rBV	13363	18402	0.70%	0.086%
2	3.211	36	38	48	rVB2	10018	15759	0.60%	0.074%
3	3.593	99	103	119	rBV	58522	99886	3.79%	0.468%
4	3.905	151	156	165	rVB	49847	68824	2.61%	0.322%
5	4.275	215	219	226	rBV8	1470	2659	0.10%	0.012%
6	4.417	239	243	248	rBV4	6265	9537	0.36%	0.045%
7	4.817	304	311	321	rVB2	12601	23101	0.88%	0.108%
8	6.775	639	644	648	rVB2	3272	4779	0.18%	0.022%
9	6.834	648	654	667	rVB	74601	134175	5.09%	0.628%
10	6.975	670	678	693	rBV	213951	336947	12.77%	1.578%
11	7.175	704	712	724	rBV	260082	441302	16.73%	2.066%
12	7.628	781	789	801	rBV	285773	458507	17.38%	2.147%
13	8.340	903	910	927	rBV	215479	400645	15.19%	1.876%
14	8.599	949	954	958	rVB7	2153	3011	0.11%	0.014%
15	8.775	976	984	994	rBV	280919	482936	18.31%	2.261%
16	9.175	1046	1052	1059	rVB2	19046	32389	1.23%	0.152%
17	9.487	1096	1105	1123	rBV	238630	437765	16.59%	2.050%
18	9.769	1147	1153	1163	rBV	1483	5018	0.19%	0.023%
19	10.028	1187	1197	1226	rBV	363567	672070	25.48%	3.147%
20	10.387	1248	1258	1267	rBV	361357	587197	22.26%	2.749%
21	10.534	1275	1283	1300	rBV	204775	408356	15.48%	1.912%
22	11.222	1393	1400	1404	rBV8	3070	6972	0.26%	0.033%
23	11.652	1466	1473	1480	rBV3	7623	14034	0.53%	0.066%
24	11.916	1511	1518	1526	rBV	104364	189186	7.17%	0.886%
25	11.981	1526	1529	1537	rVB4	6486	13131	0.50%	0.061%
26	13.663	1807	1815	1832	rBV	646891	1035690	39.26%	4.849%
27	13.940	1855	1862	1875	rBV	812465	1135845	43.05%	5.318%
28	14.251	1909	1915	1923	rBV	684986	889451	33.72%	4.164%
29	14.534	1957	1963	1974	rBV2	35089	95556	3.62%	0.447%
30	14.728	1993	1996	2001	rVB7	4826	8140	0.31%	0.038%
31	15.275	2079	2089	2095	rBV	1087467	1559265	59.10%	7.300%
32	15.322	2095	2097	2104	rVB4	11796	17775	0.67%	0.083%
33	15.422	2106	2114	2126	rBV	280452	460173	17.44%	2.154%
34	16.228	2246	2251	2254	rBV7	2469	4099	0.16%	0.019%
35	16.722	2333	2335	2341	rVB6	2165	3473	0.13%	0.016%
36	17.063	2387	2393	2404	rVV	895698	1175270	44.55%	5.502%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022774.D
 Acq On : 31 Oct 2024 17:40
 Operator : RC/JU
 Sample : P4630-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	17.163	2404	2410	2423	rVV2	1190441	1907731	72.31%	8.932%
38	17.645	2488	2492	2496	rBV6	1971	3610	0.14%	0.017%
39	17.763	2507	2512	2516	rBV7	2872	4638	0.18%	0.022%
40	17.998	2547	2552	2558	rBV2	30009	44263	1.68%	0.207%
41	18.075	2562	2565	2570	rVB2	5272	6468	0.25%	0.030%
42	19.104	2736	2740	2745	rBV3	17612	23981	0.91%	0.112%
43	19.175	2749	2752	2756	rVV	19614	26362	1.00%	0.123%
44	19.222	2756	2760	2767	rVV4	33101	51557	1.95%	0.241%
45	19.334	2775	2779	2788	rBV5	29645	45037	1.71%	0.211%
46	19.551	2811	2816	2825	rBV	1756429	2323947	88.09%	10.880%
47	21.504	3142	3148	3160	rVB2	857680	1446780	54.84%	6.774%
48	24.545	3656	3665	3679	rVB	1069609	2638137	100.00%	12.351%
49	24.763	3694	3702	3718	rVB	585126	1585020	60.08%	7.421%


Sum of corrected areas: 21358856

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022774.D
Acq On : 31 Oct 2024 17:40
Operator : RC/JU
Sample : P4630-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

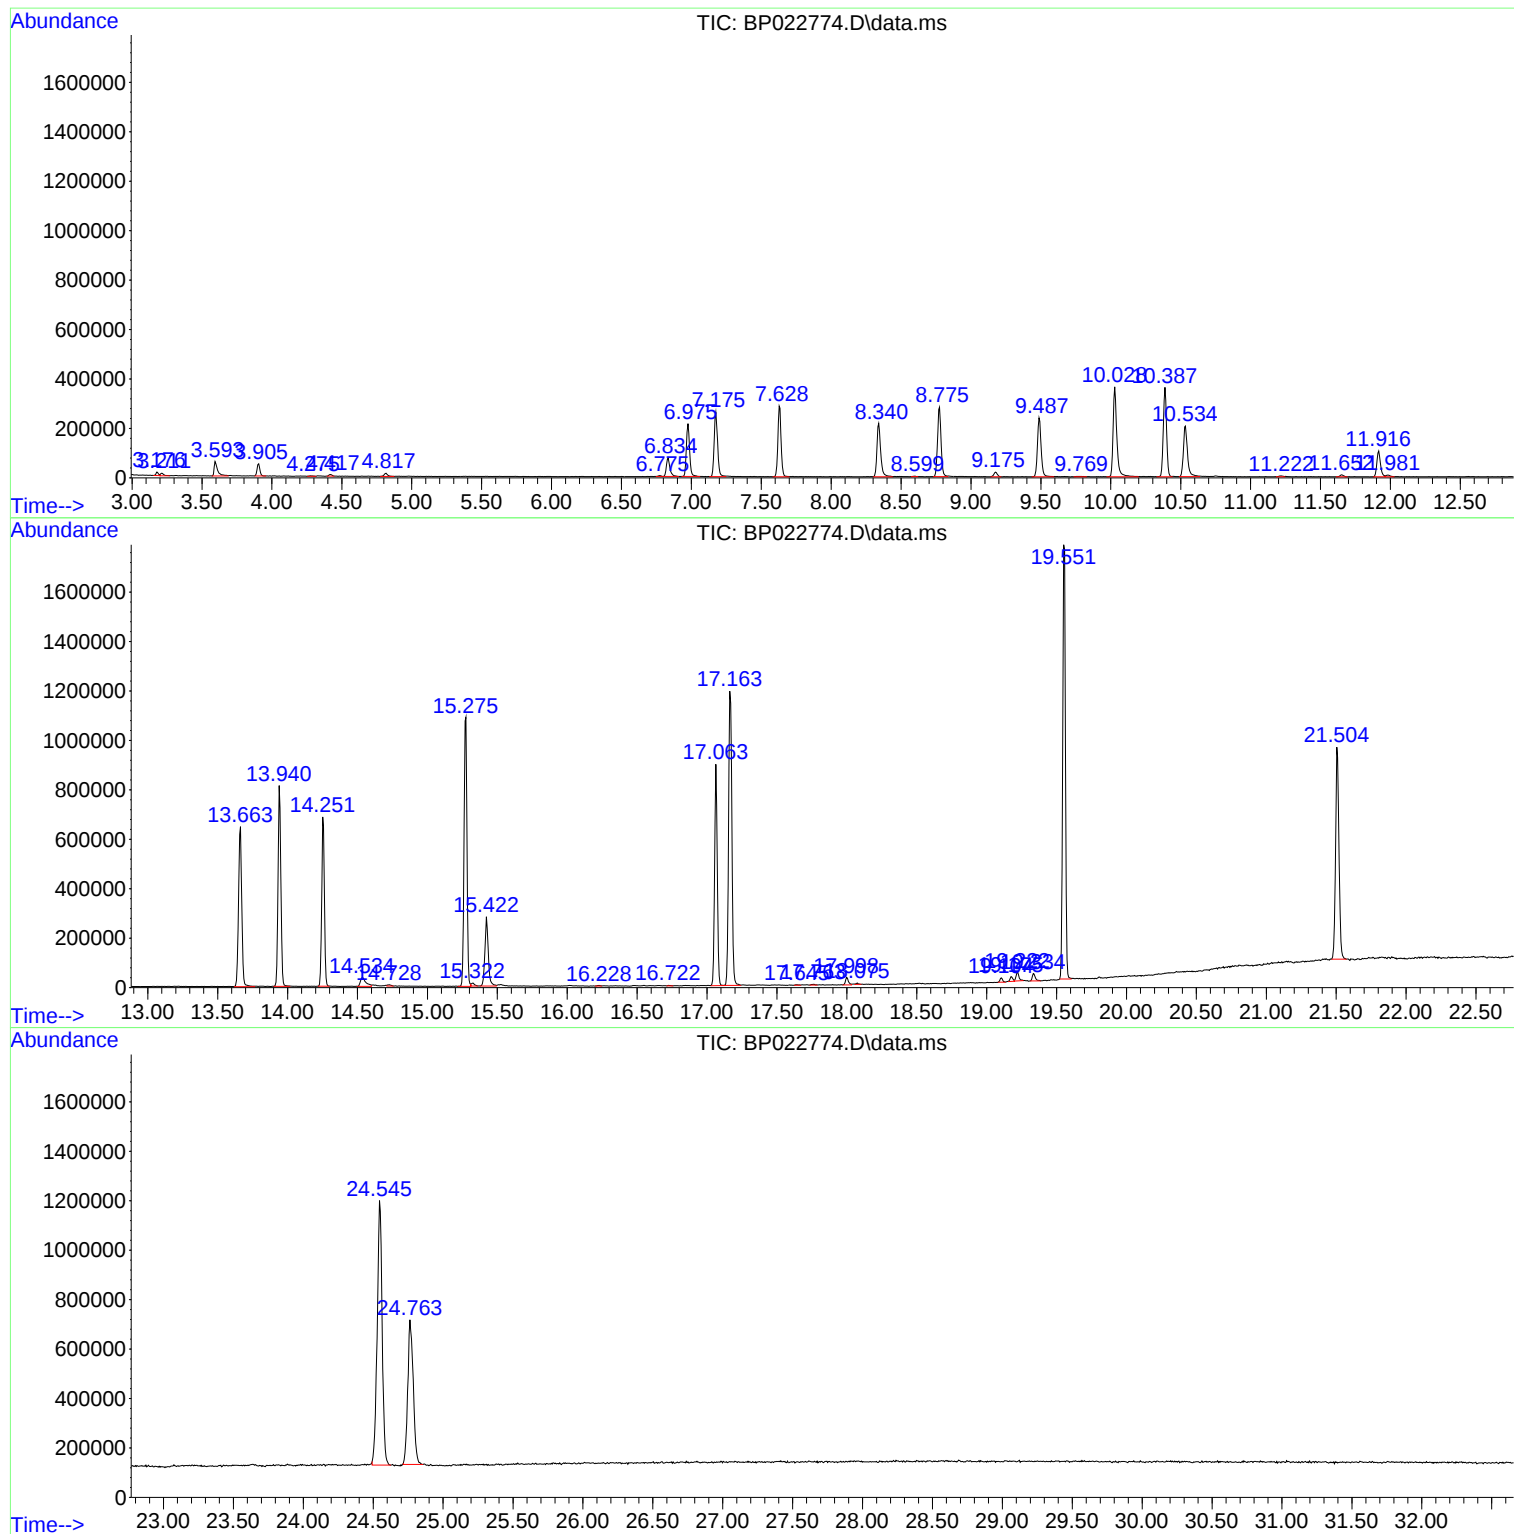

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022774.D
Acq On : 31 Oct 2024 17:40
Operator : RC/JU
Sample : P4630-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Toluene Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.905	3.00 ng/ul	68824	1,4-Dichlorobenzene-d4	7.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Toluene	92	C7H8	000108-88-3	90
2			Spiro[2,4]hepta-4,6-diene	92	C7H8	000765-46-8	90
3			Toluene	92	C7H8	000108-88-3	90
4			Toluene	92	C7H8	000108-88-3	87
5			Toluene	92	C7H8	000108-88-3	87

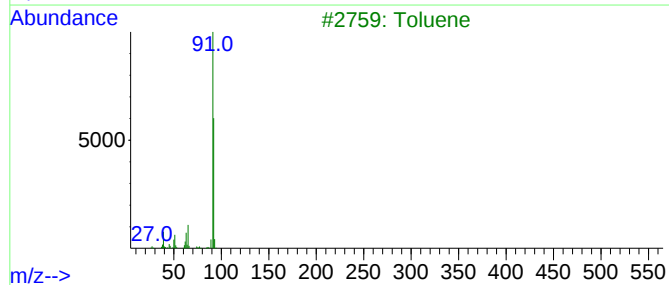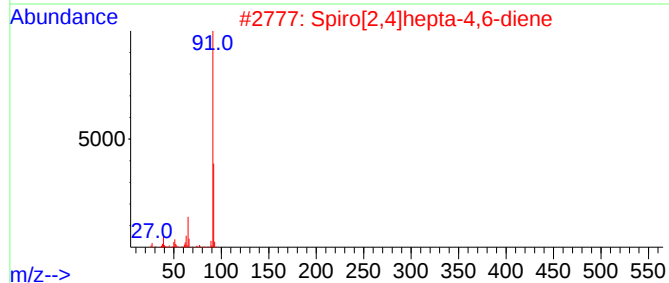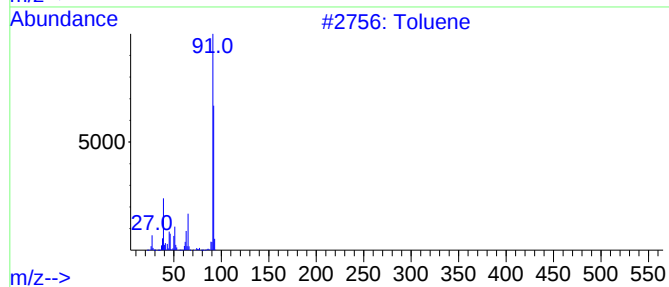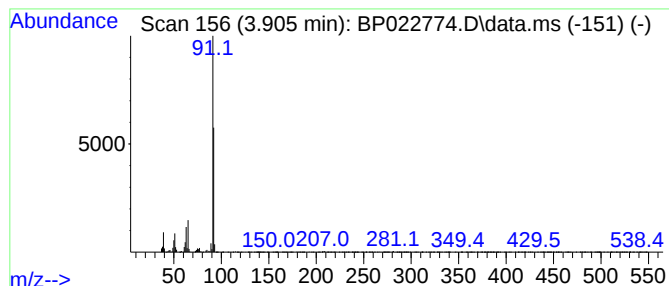

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022774.D
Acq On : 31 Oct 2024 17:40
Operator : RC/JU
Sample : P4630-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Toluene	3.905	3.0	ng/ul	68824	1	7.628	458507	20.0